

# Particle accelerators and their medical applications

**Varchaswi K S Kashyap**

School of Physical Sciences

National Institute of Science Education and Research (NISER)  
Bhubaneswar

*Have you come across any particle accelerators in your daily life?*


# What about these?



**CRT television**




**CRT monitor**

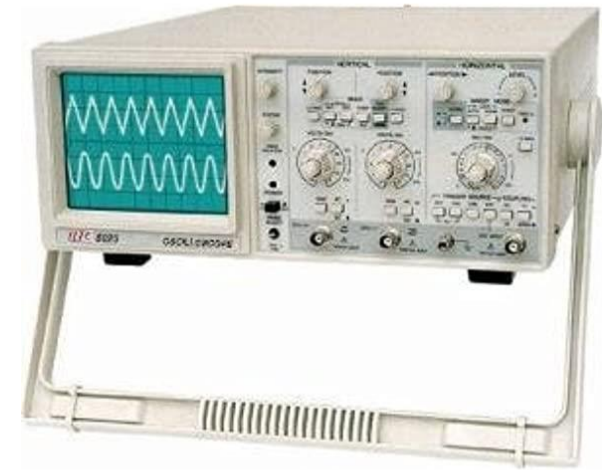

**CR Oscilloscope**

They have small accelerators that can accelerate electrons up to few keV

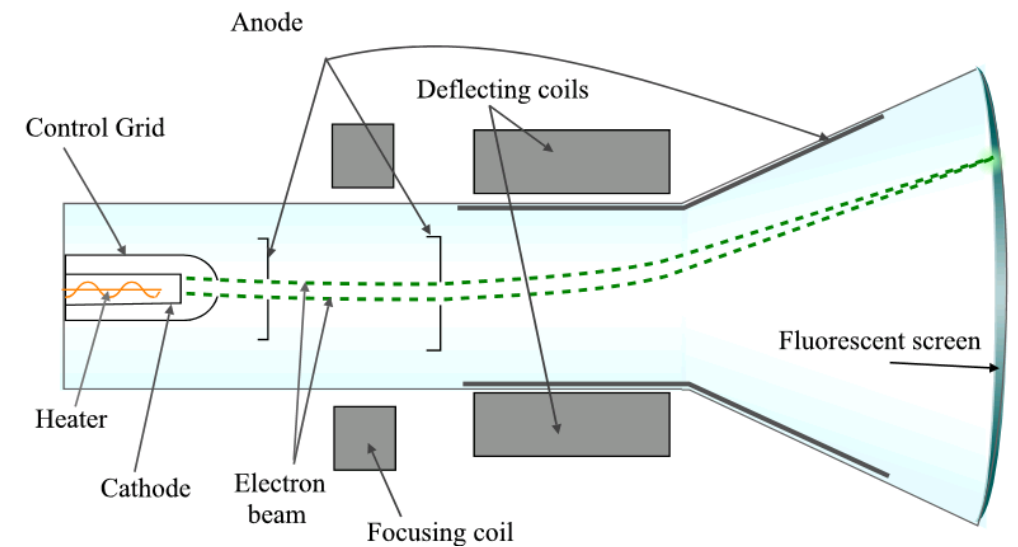

# Need for accelerators in physics

- Development of accelerators was driven by the curiosity to probe more and more in to the constituents of matter
- De Broglie's principle is what guides the energy of particles needed to probe into matter

$$\lambda = \frac{h}{p}$$

Dimension to be probed	1 Å (Atomic size)	1 fm (Nuclear size)
Energy of electron required	~150 eV	~ 1 TeV

Where  $\lambda$  is the wavelength,  $h$  is the Planck's constant and  $p$  is the momentum.

- Larger the momentum (Energy), lower is the wavelength and hence smaller is the object that can be probed

# Types of accelerators

## Electrostatic accelerators

- Cockroft – Walton accelerator
- Van de Graaff accelerator
- Pelletron


## Induction accelerators

- Induction Linear accelerator
- Betatron

## Radio-Frequency (RF) accelerators

- **RF Linac**
- RF quadrupole
- **Cyclotron**
- Microtron
- **Synchrotron**

# Cockroft – Walton accelerator

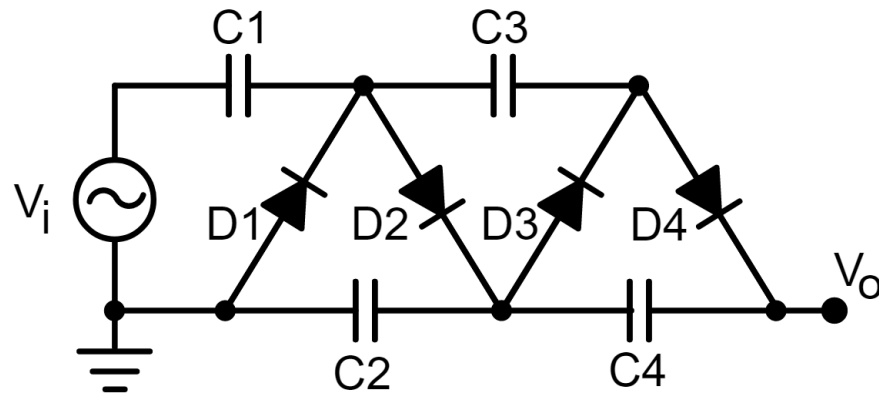


- Converts AC voltage to very high DC voltage
- Simple in principle and less bulky compared to transformers
- Voltages can be tapped at different levels

$$\text{K.E.} = qV$$

*Source: Wikipedia*



# Van de Graaff accelerator

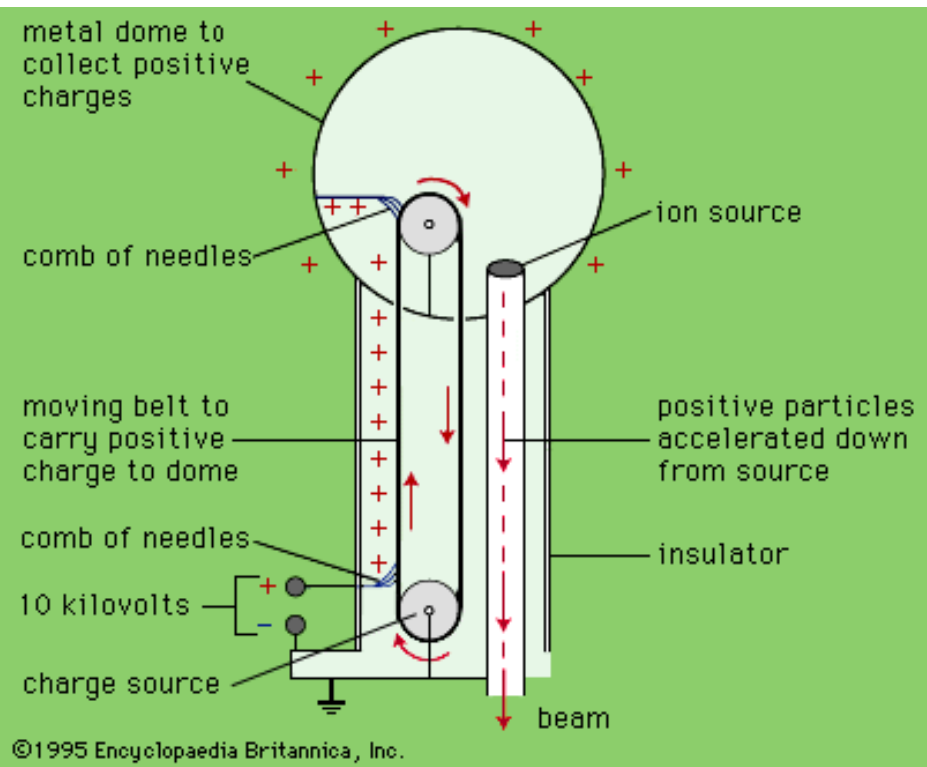


A Van de Graaff particle accelerator in a pressurized tank at Pierre and Marie Curie University, Paris (Source: Wikipedia, Copyright © 2004 David Monniaux)


- Voltages of the order of a few MV can be achieved.
- A high voltage supply provides charges to be transported to the metal dome
- Charges are collected in a metal dome over time
- The potential difference between the dome and the ground can be used to accelerate particles
- A Pelletron is very similar to the Van de Graaff having a metal belt with pellets instead of a rubber belt.

$$K.E. = qV$$


# Linear accelerator

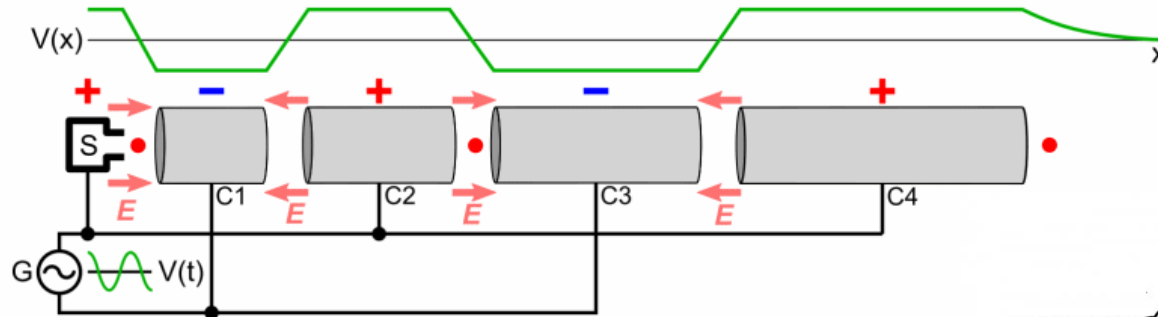

RF LINAC (Image credit: Wikipedia)

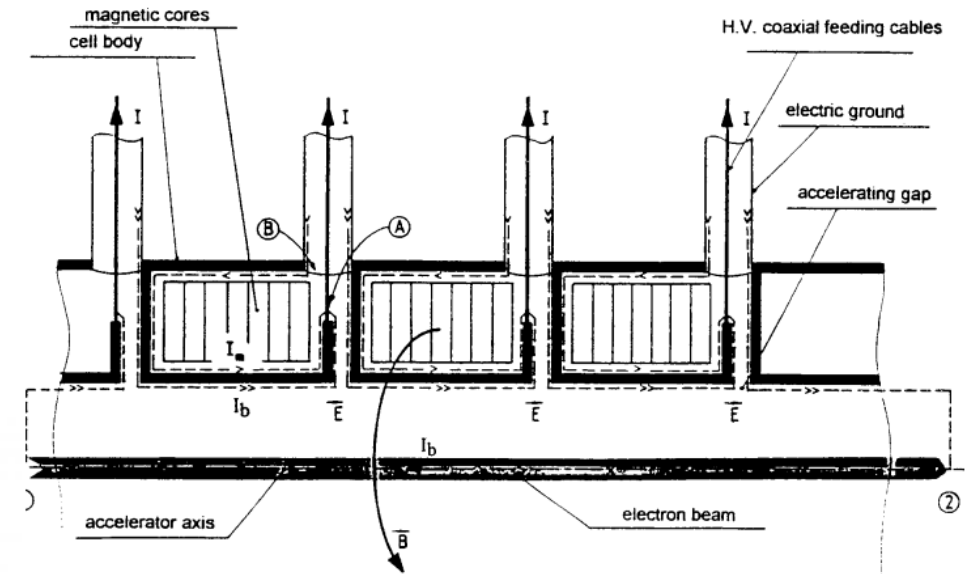

INDUCTION LINAC (Image credit: INDUCTION, J De Mascureau, 1996)

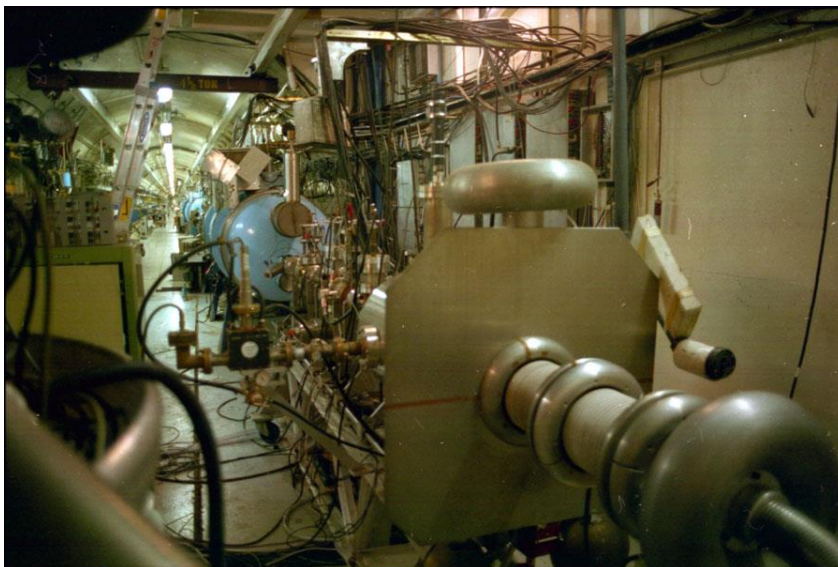


The [Stanford University](#) superconducting linear accelerator, housed on campus below the Hansen Labs until 2007. This facility is separate from [SLAC](#) (Image credit: Wikipedia)

RF LINAC	INDUCTION LINAC
Smaller length	Longer length
Higher acceleration gradient	Lower acceleration gradient
Requires lower power	Requires higher power
Low current and short pulse duration	High current and longer pulse duration




# Linear accelerator (LINAC) contd.

## RF LINAC configurations

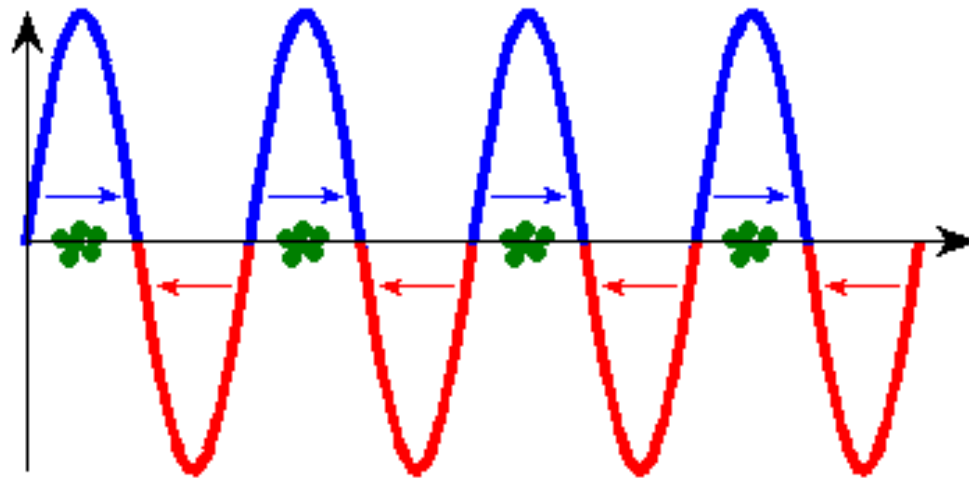


Standing wave

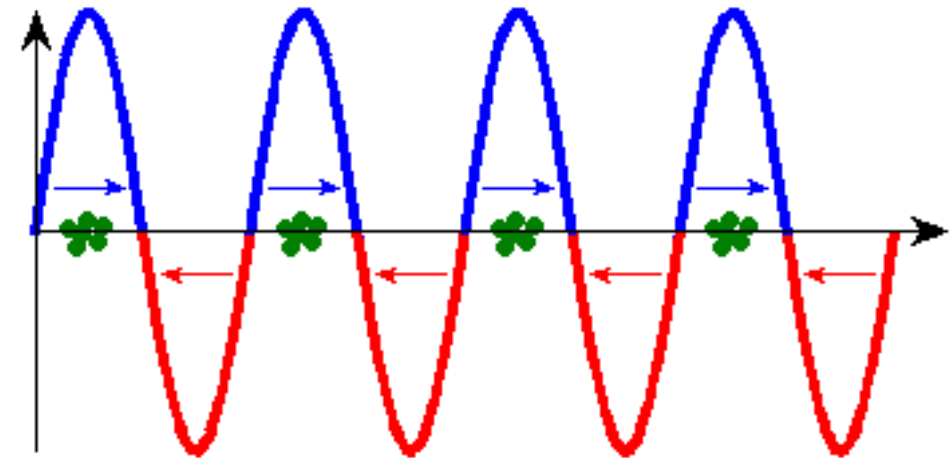

Travelling wave


**Image credit:** By Patrick87 - <https://commons.wikimedia.org/w/index.php?curid=29590284>

# Medical LINAC

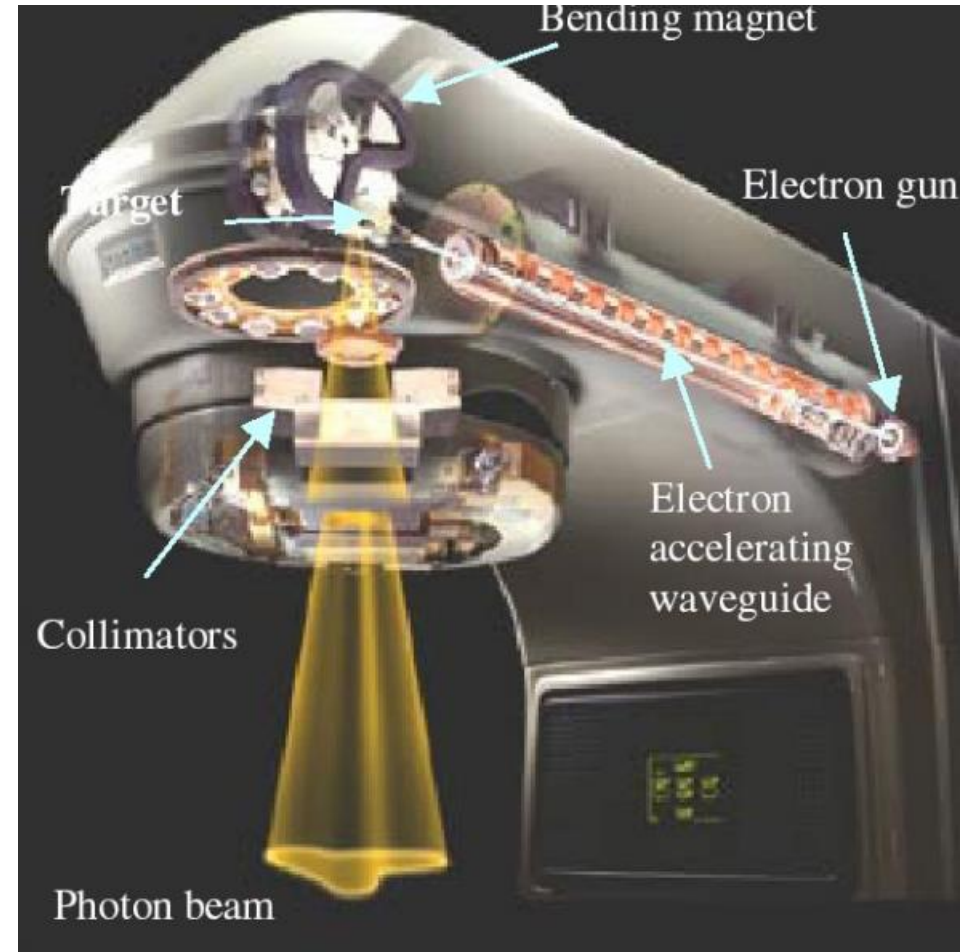


**Image credit:** Medical Linear Accelerators in Radiation Therapy, Presentation by Haijun Song, Ph.D. Dept. of Radiation Oncology Duke University Medical Center

# Medical LINAC configurations

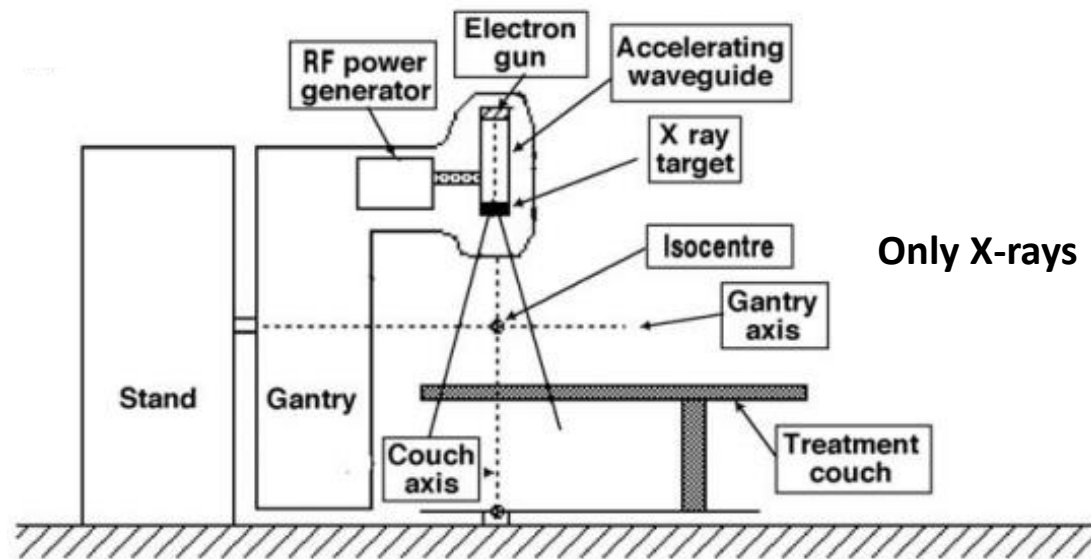


Only X-rays

RF power generator and waveguide are both in the gantry and the waveguide is directed straight towards the patient

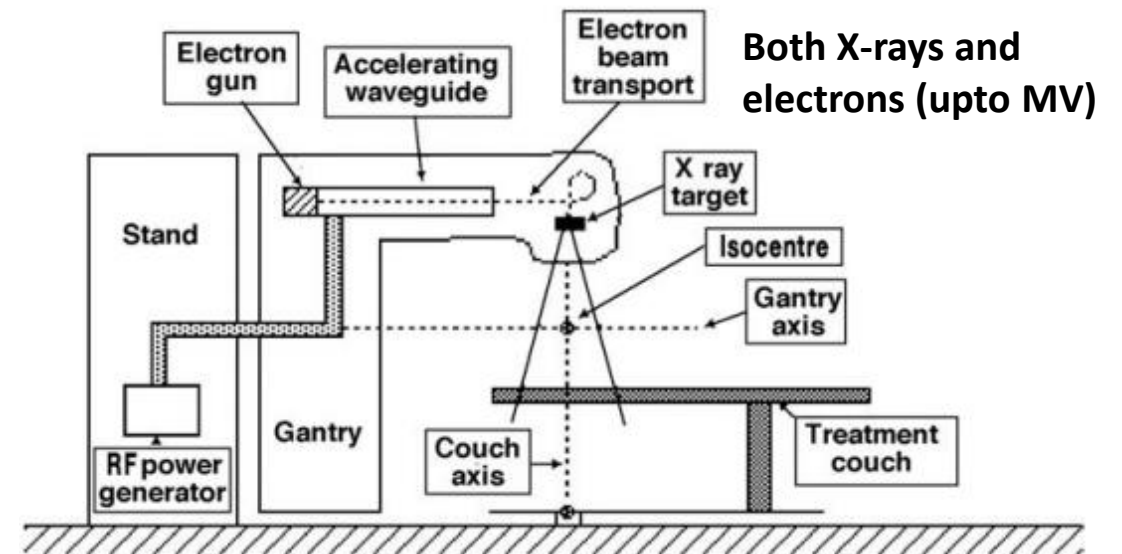

Both X-rays and electrons (upto MV)

RF power generator is in the gantry stand and waveguide is in the gantry directed towards the target above the patient

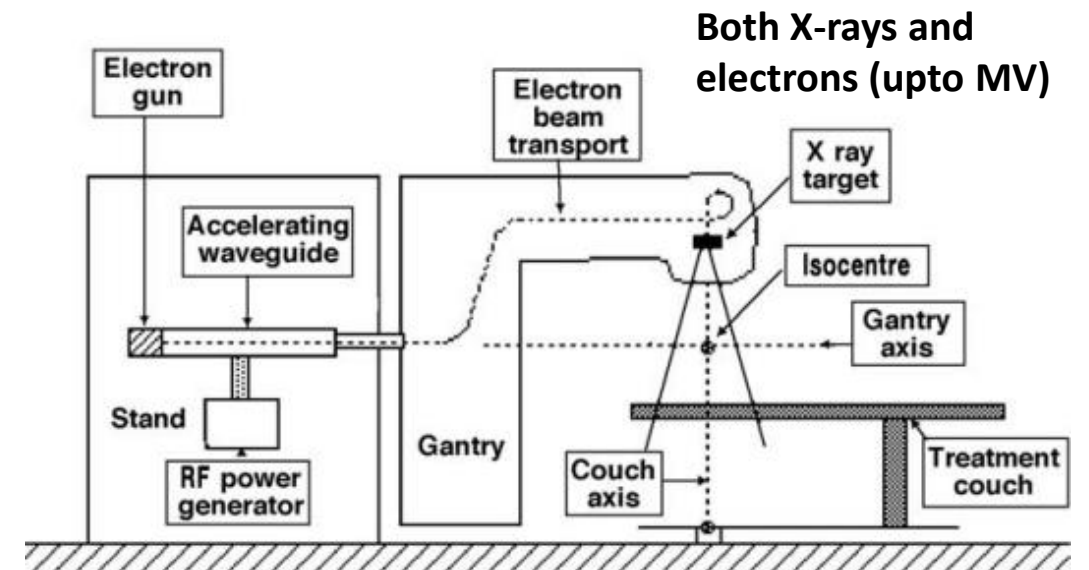


Both X-rays and electrons (upto MV)

Both RF power generator and waveguide are in the gantry stand. The electrons have to be transported to the target.

Image credit: Treatment machines for external beam radiotherapy, E.B. Podgorsak, Department of Medical Physics, McGill University Health Centre, Montreal, Quebec, Canada

# Medical LINAC configurations contd.

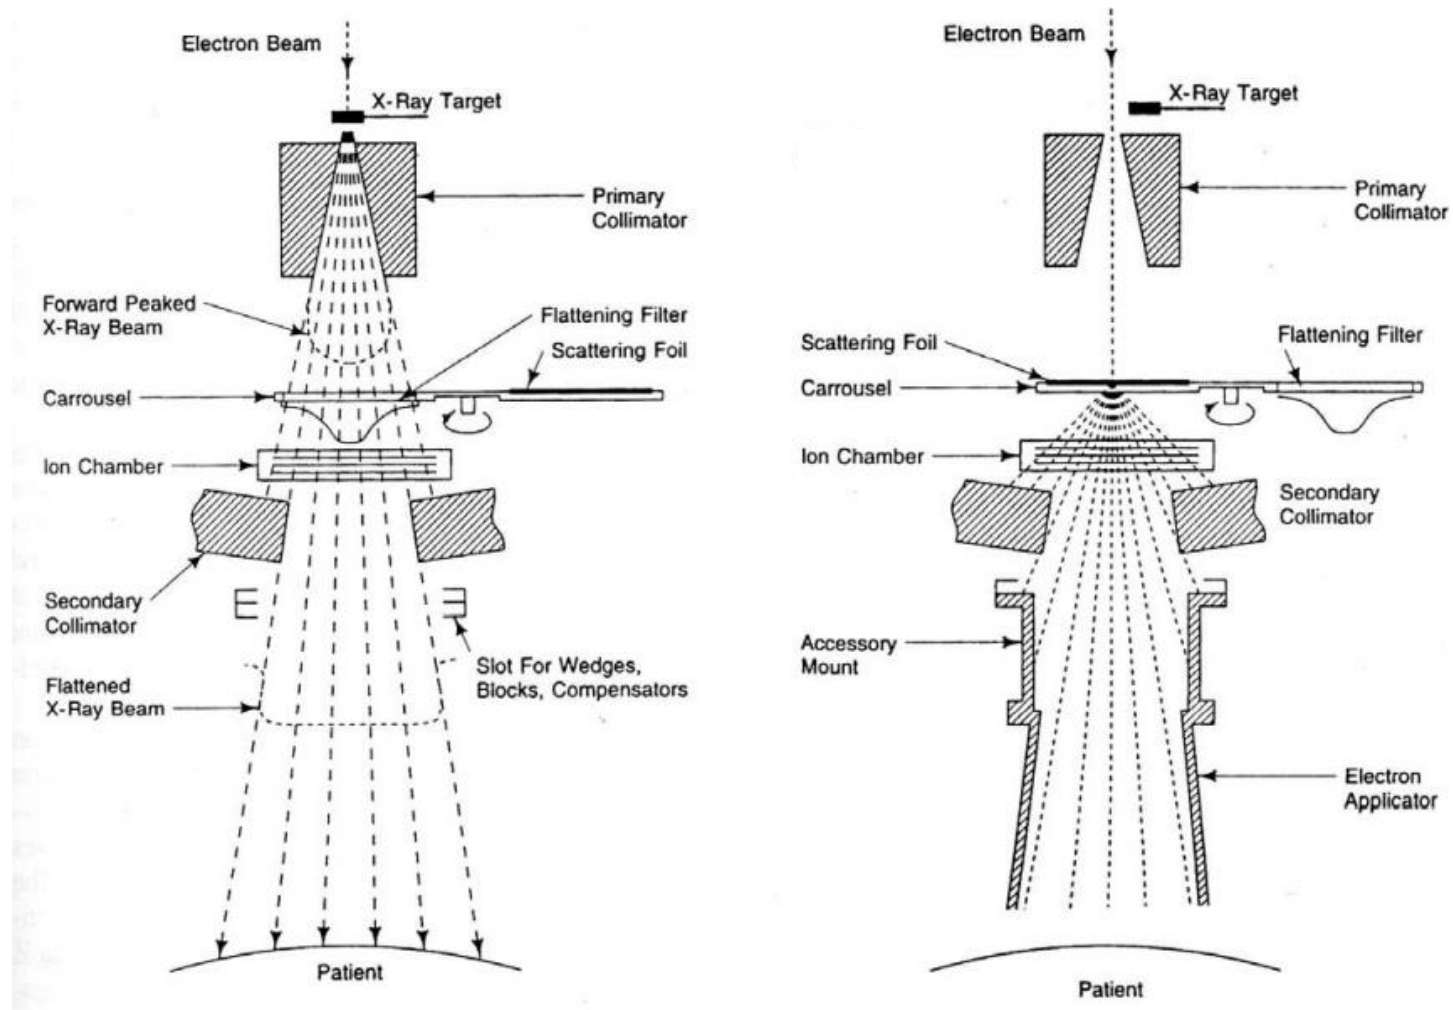

**Image credit:**  
Medical Linear Accelerators in Radiation Therapy, Presentation by Haijun Song, Ph.D. Dept. of Radiation Oncology Duke University Medical Centre

# Cyclotron

$$T = \frac{2\pi m}{Bqv}$$

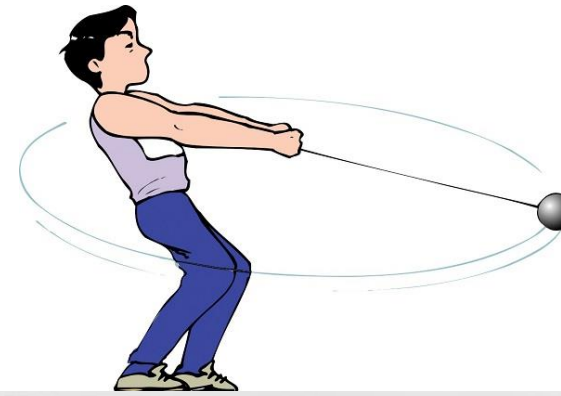


Image credit:  
[Hammer Throw -  
How to Play?  
\(tutorialspoint.co  
m\)](https://www.tutorialspoint.com)


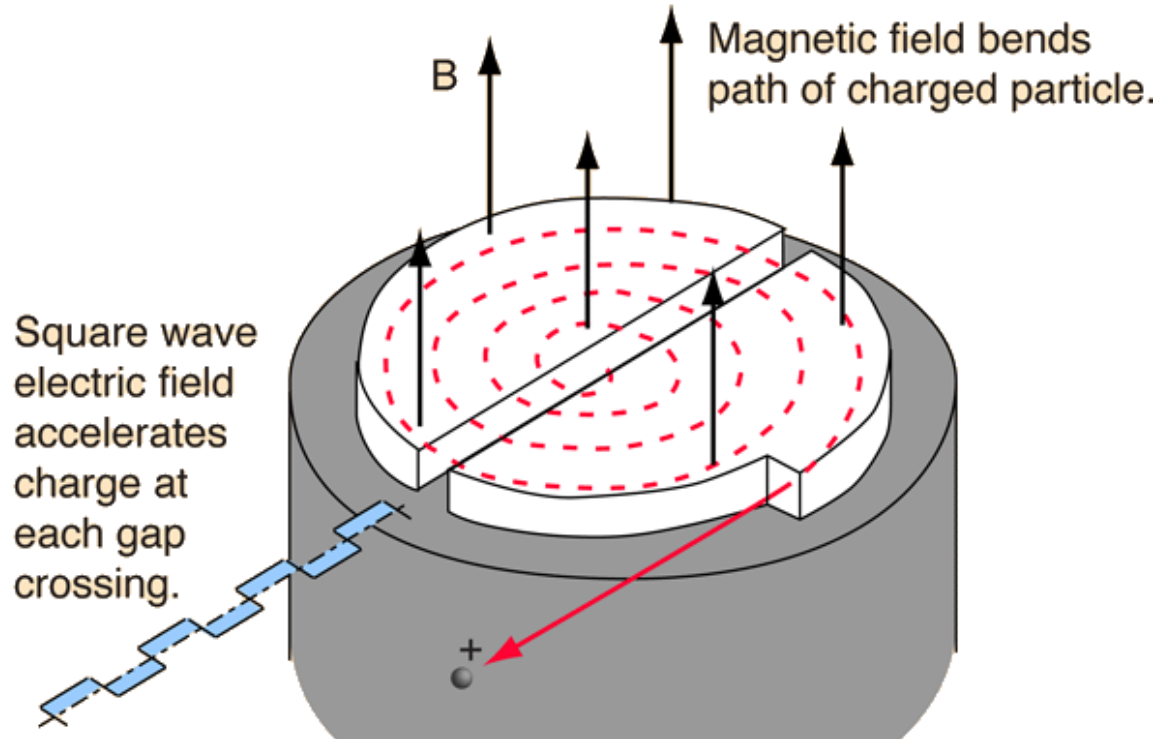


Image credit: [Cyclotron \(gsu.edu\)](https://www.gsu.edu)

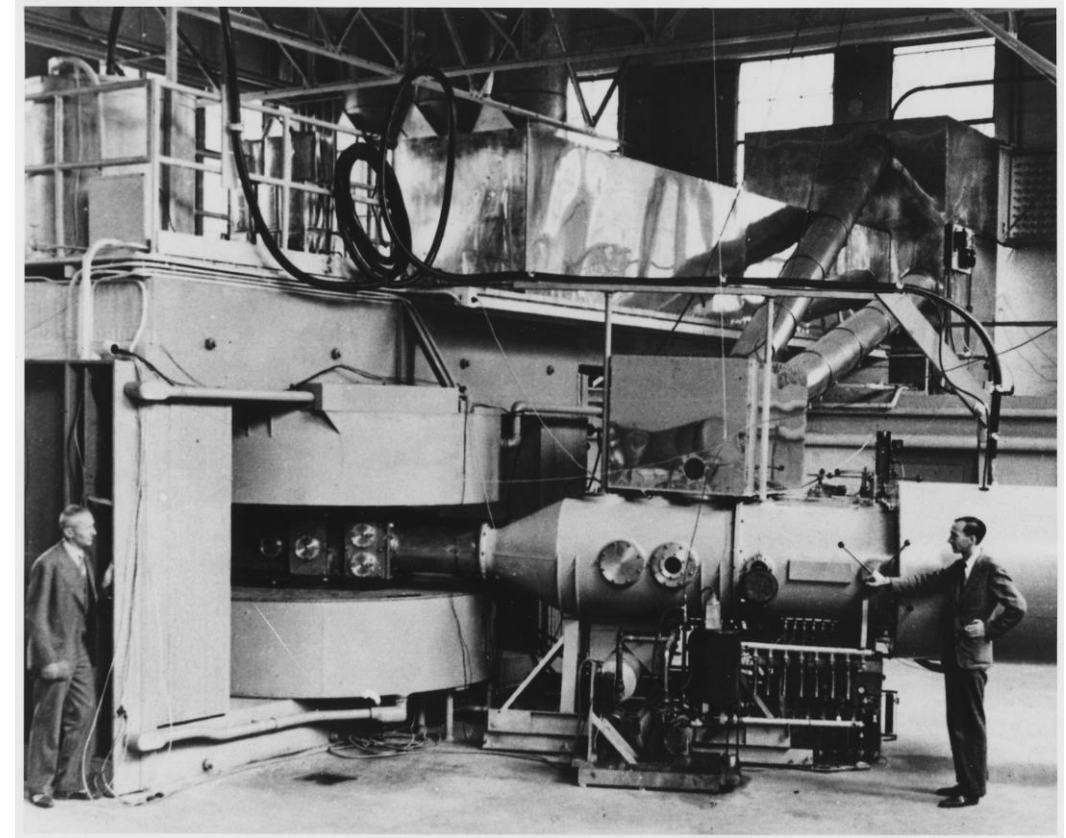

Lawrence's 60-inch cyclotron, with magnet poles 60 inches (5 feet, 1.5 meters) in diameter, at the [University of California Lawrence Radiation Laboratory](https://www.lawrenceberkeley.gov/), Berkeley, in August, 1939. Image credit: Wikipedia

# What to do if particle becomes relativistic?

## Iso-cyclotron (Isochronous)

Keep frequency constant and vary the magnetic field



Image credit:  
[COMET Cyclotron | CPT | Paul Scherrer Institut \(PSI\)](#)

## Synchro-cyclotron

Keep magnetic field constant and vary the frequency

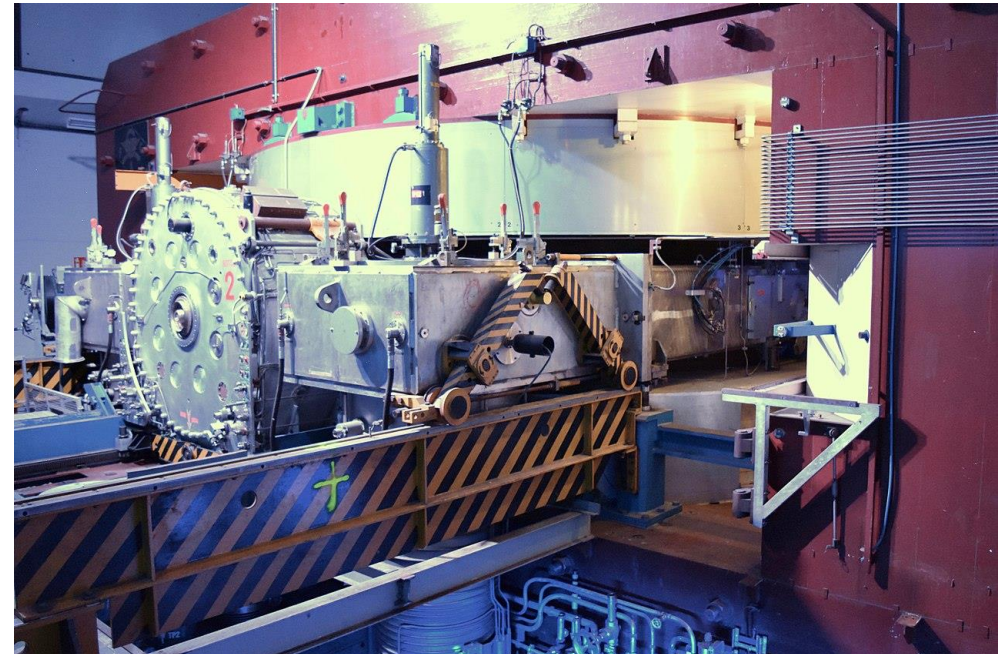


Image source: Wikipedia

# What to do if particle becomes relativistic?

## Iso-cyclotron (Isochronous)

Keep frequency constant and vary the magnetic field

Alias: Azimuthal varying field cyclotron

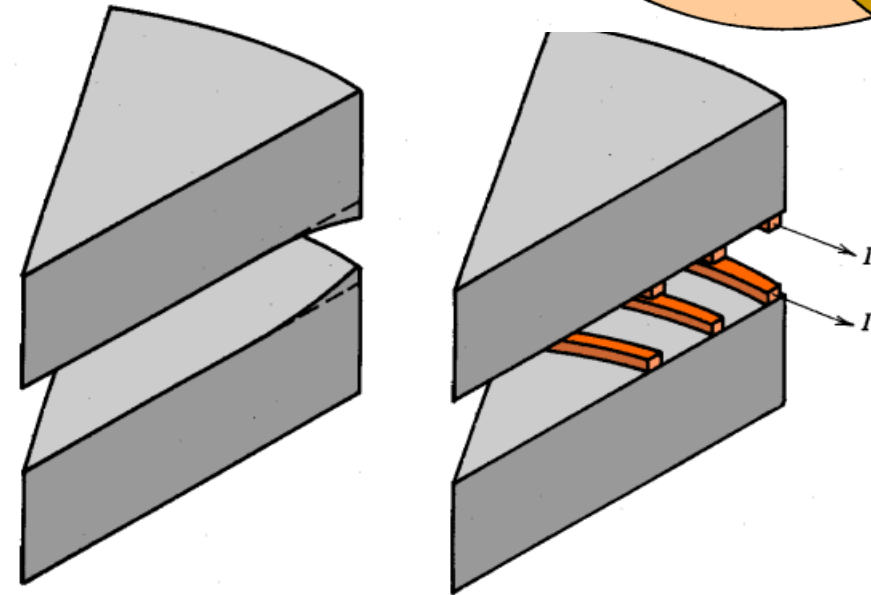
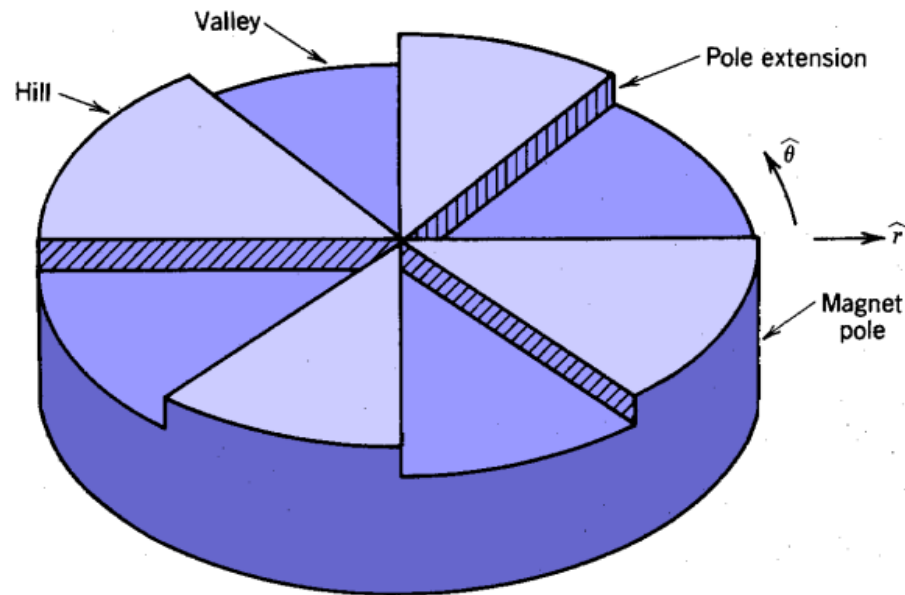
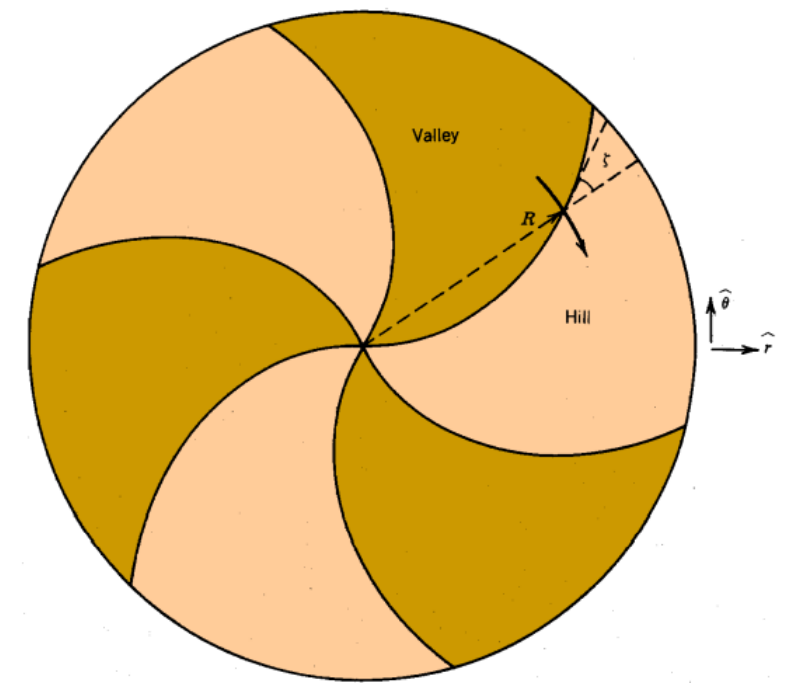


Image credit: <http://www.geology.wisc.edu/~johnf/g777/Misc/chap15.pdf>

# What to do if particle becomes relativistic?

- Higher energy achievable
- Lower average beam current
- Compact dimension

## Synchro-cyclotron

Keep magnetic field constant and vary the frequency

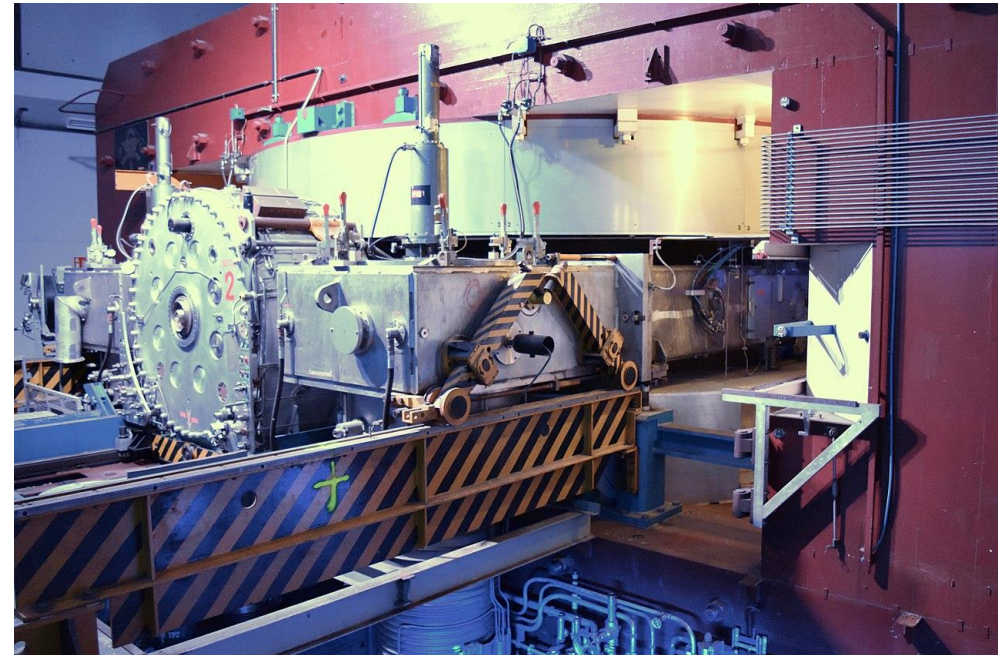


Image credit: Wikipedia



# Layout of a cyclotron complex for proton therapy

## PSI

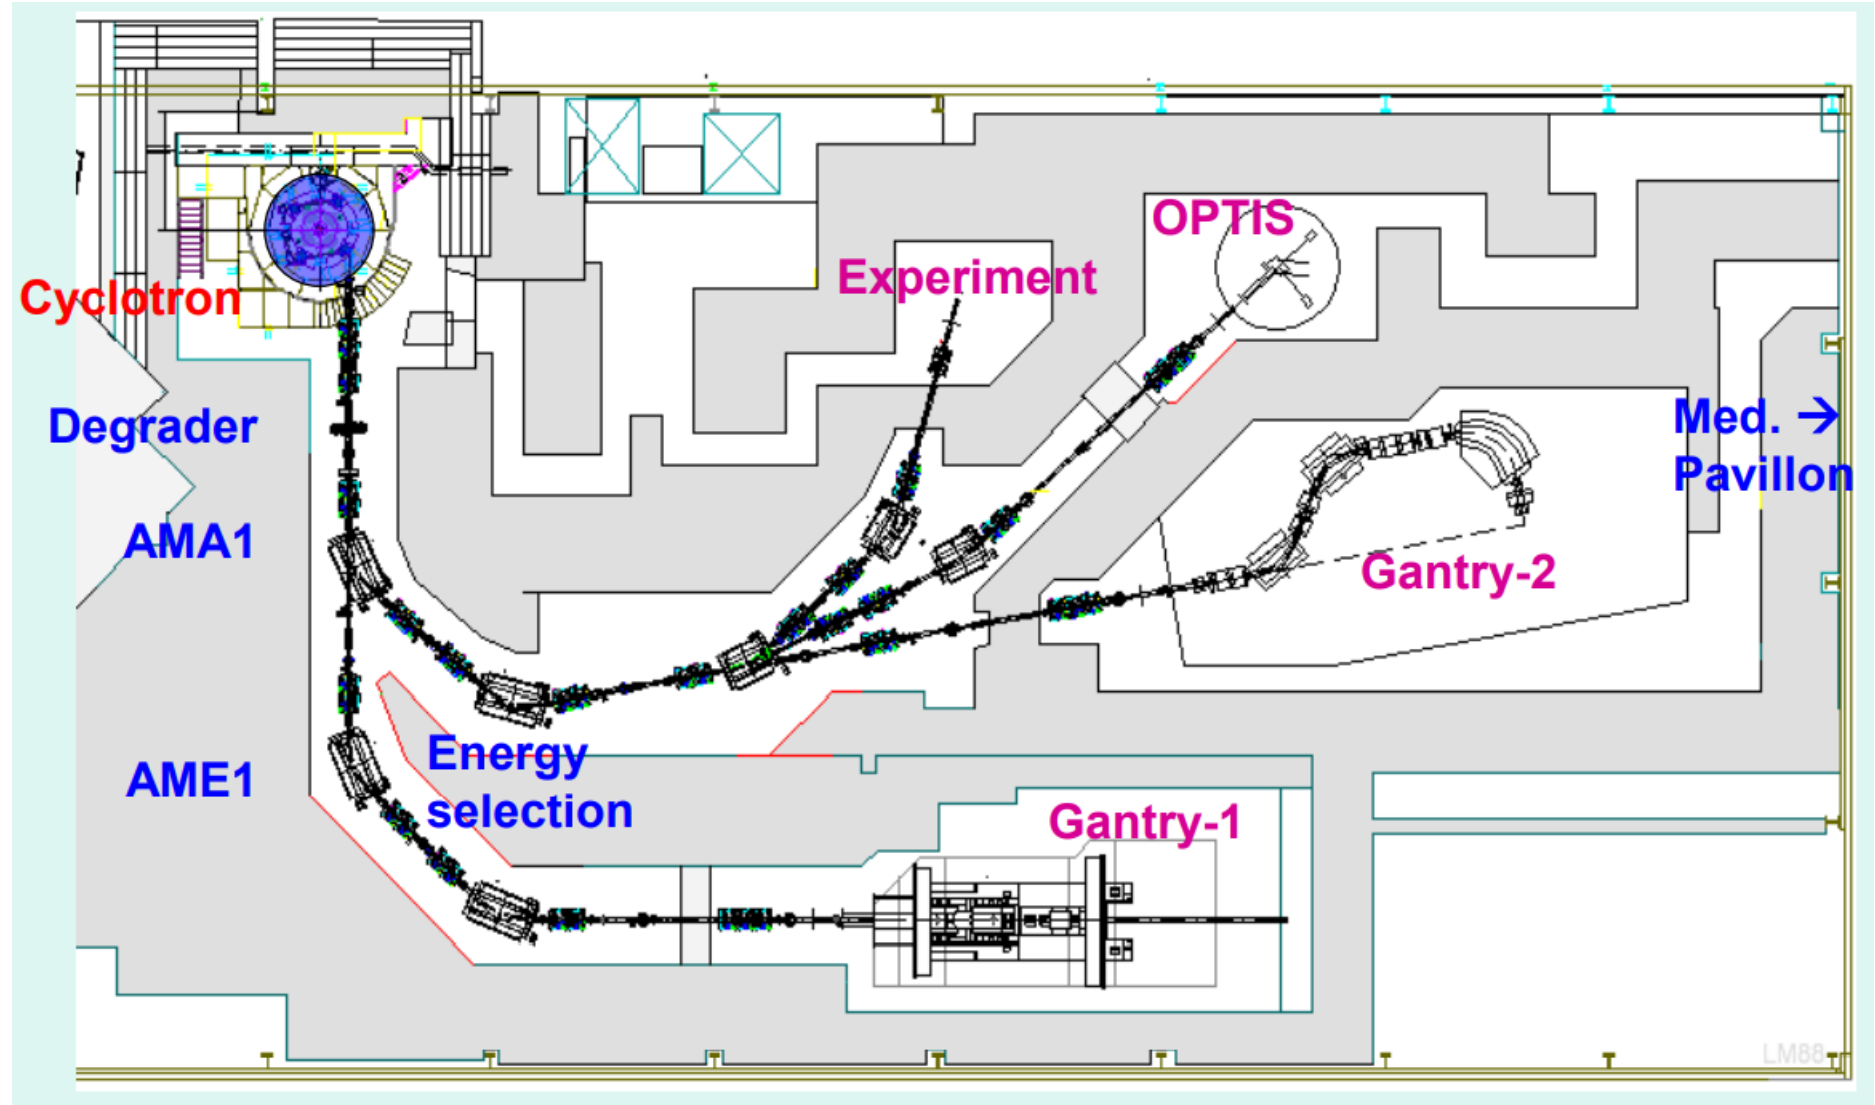


Image credit: Accelerators for proton therapy, Presentation by, Marco Schippers, PSI - JUAS

What if both the frequency and magnetic field can be changed?

# Synchrotron

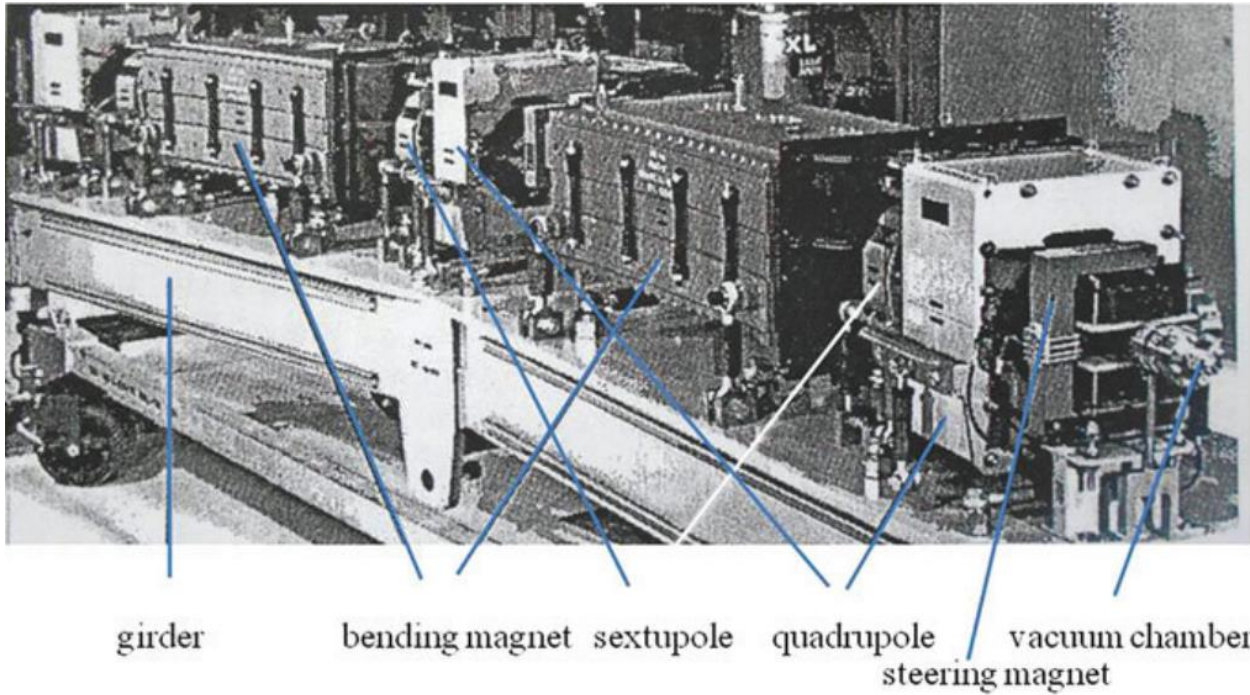


Image credit: Particle Accelerator Physics, Helmut Wiedemann, 4<sup>th</sup> edition, Springer

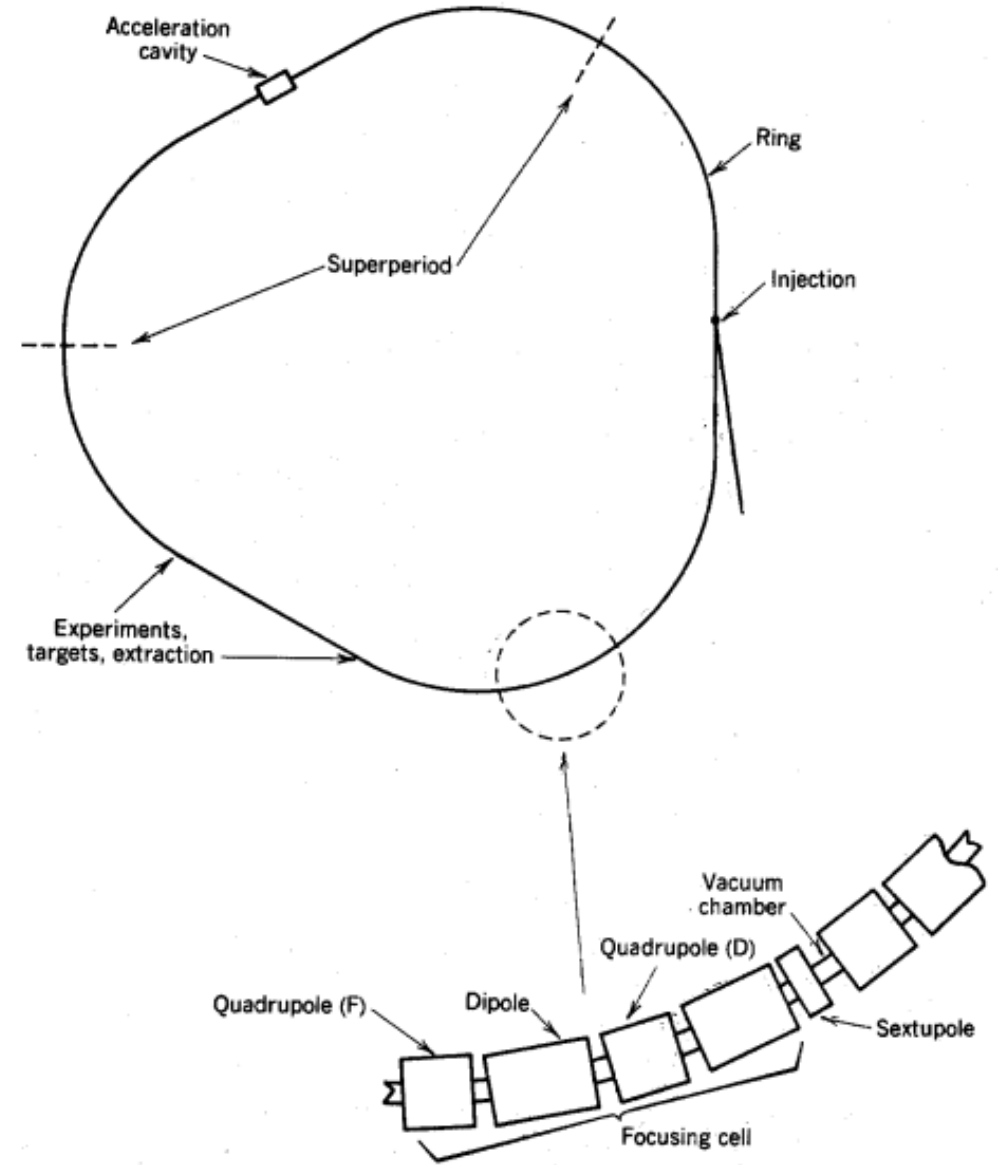



Image credit:  
<http://www.geology.wisc.edu/~johnf/g777/Misc/chap15.pdf>

# Particle accelerators and medical use

Particle	Accelerator	Energy	Use
Electron	LINAC	~6-25 MeV	Cancer treatment
X-rays	LINAC	~6 MeV	Cancer treatment
	Synchrotron	~100s of keV	Imaging - coronary angiography, bronchography, mammography, computed tomography, x-ray microscopy
Proton	Cyclotron	~20-100 MeV	Radioactive assay preparation for PET, SPECT scanning
	Synchrocyclotron	~250 MeV	Cancer treatment
Carbon	Synchrotron	~400 MeV/u	Cancer treatment


Have I missed a very important part?

# Particle sources?

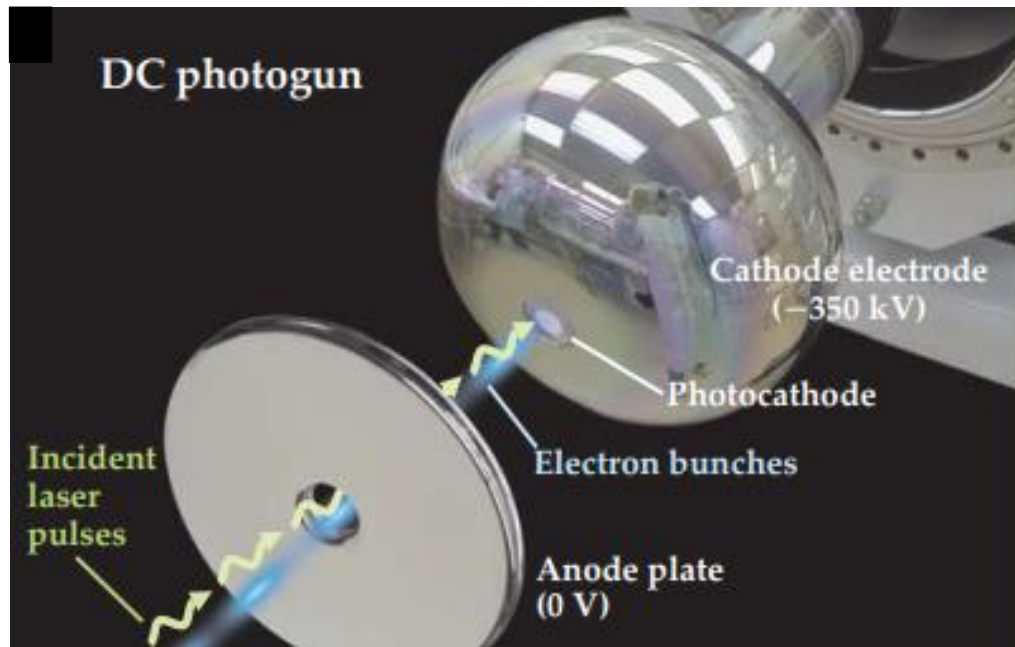

## Photocathode based electron source.

**Image credit:** Electron sources for accelerators Carlos Hernandez-Garcia, Patrick G. O'Shea, and Marcy L. Stutzman, Physics Today, February 2008 (Volume 61, Issue 2).

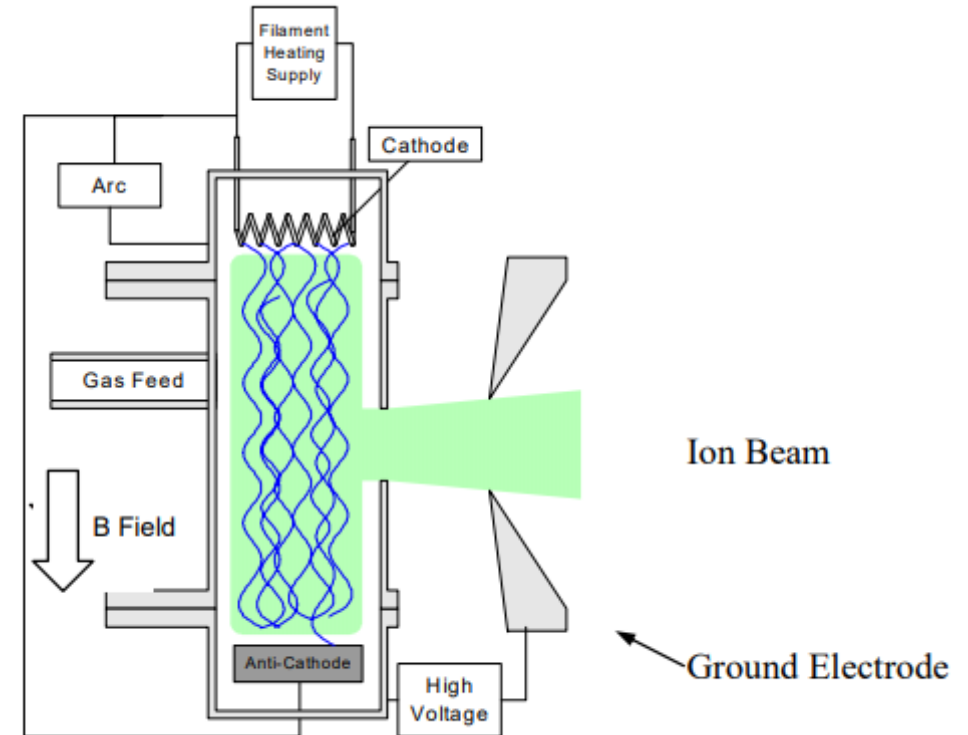

## Penning ion source

**Image source:** electron and ion sources for particle accelerators R. Scrivens

Thank you.

*Hope you've all been accelerated!!*