

Online beam monitoring detector for FLASH irradiations



Paula Ibáñez García

Grupo de Física Nuclear & IPARCOS, Universidad
Complutense de Madrid


Instituto de Investigación Sanitaria del Hospital Clínico San
Carlos

Miguel García Díez, Andrea Espinosa, Víctor Sánchez -Tembleque, Daniel
Sánchez-Parcerisa, Víctor Valladolid, Juan A. Vera, Alejandro Mazal, Luis Mario
Fraile, José Manuel Udías

CONVENTIONAL -RT

Dose/fraction: **1-2 Gy**
Delivery time ~ **days/weeks.**

0 Gy

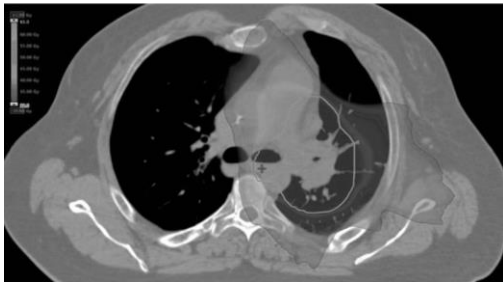


0.01-0.1 Gy/s

FLASH-RT

Dose/fraction: **10-40 Gy**
Delivery time ~ **μ s - ms**

0 Gy

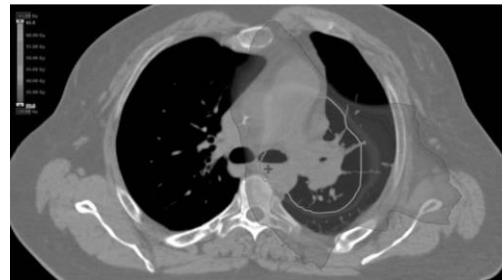

> 40 Gy/s

FLASH effect:

1. Reduced radiation-induced damage in healthy tissue
2. Similar antitumor effectiveness



1a : Day 0



1b : 3 weeks




1c : 5 months


FLASH Effect

• Deeply influenced by beam pulse structure


- Average dose rate
- Dose rate in the pulse
- Pulse repetition frequency
- Dose per pulse

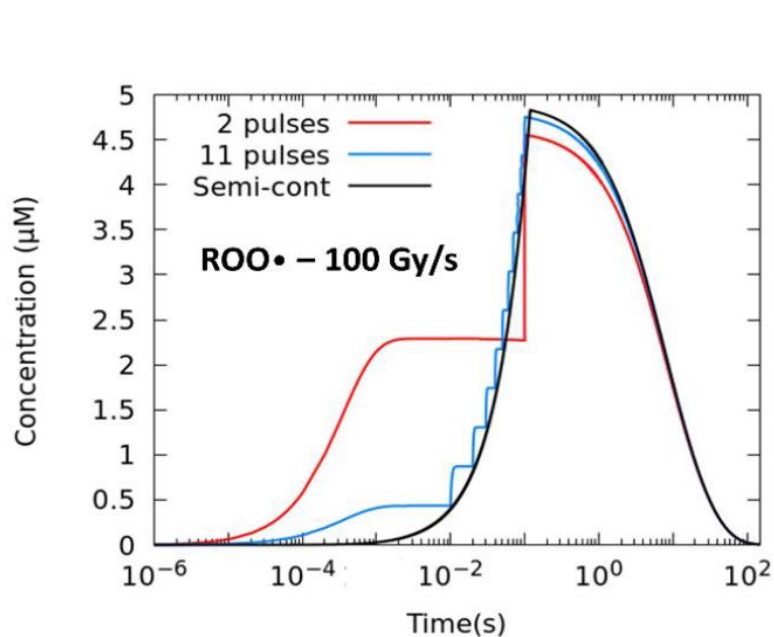

Time evolution of the ROO• radical for different degrees of pulsatility (10 Gy)

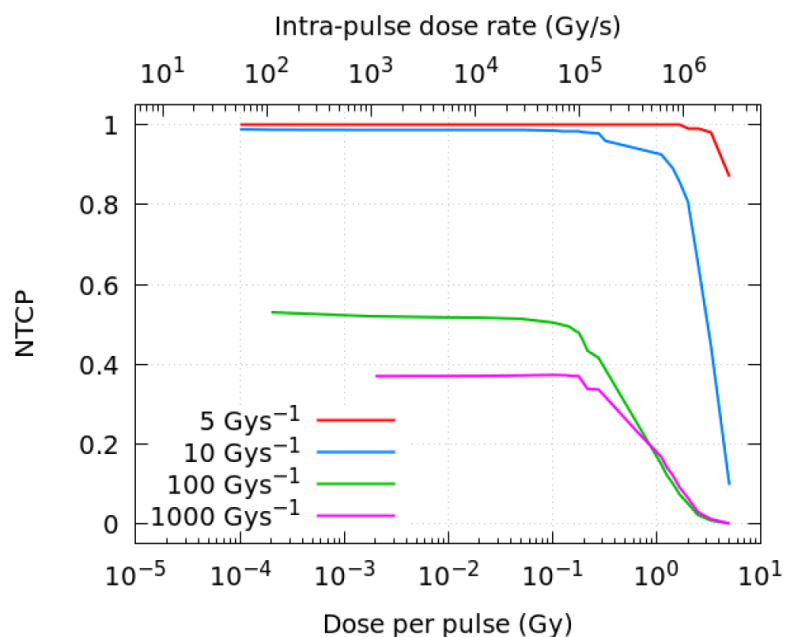

NTCP vs dose per pulse for different mean dose rates (10 Gy)

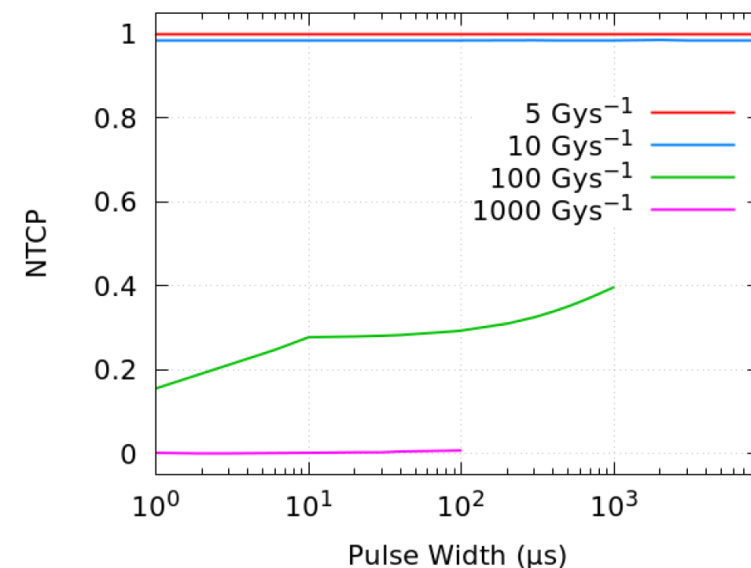


NTCP vs pulse width for different mean dose rates (10 Gy)

Espinosa-Rodríguez et al. Int. J. Mol. Sci. 2022, 23, 13484

FLASH Effect

- Deeply influenced by beam pulse structure
 - Average dose rate
 - Dose rate in the pulse
 - Pulse repetition frequency
 - Dose per pulse

Fast and accurate monitoring of the time structure is vital for FLASH treatments

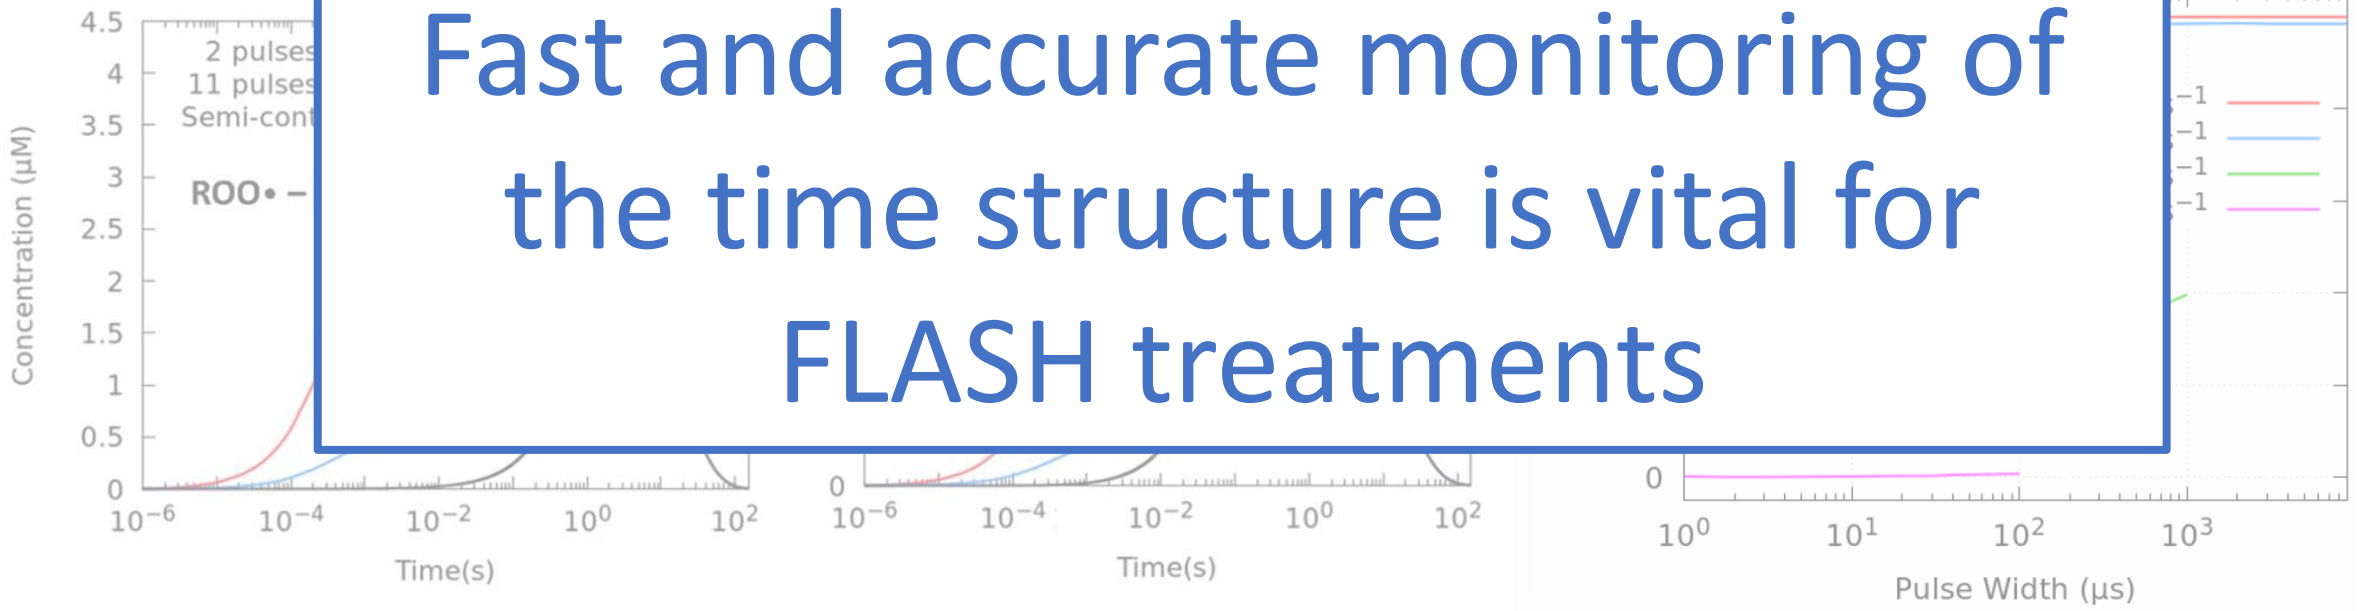

Time evolution of the ROO• radical for different degrees of pulsatility

NTCT vs pulse width for different mean dose rates


Espinosa-Rodríguez et al. Int. J. Mol. Sci. 2022, 23, 13484

Online beam monitoring detector. FLASH irradiations

Requirements:

- Extended dynamic range
- High temporal resolution
- Radiation hardness

Radiochromic film dosimetry & TLD

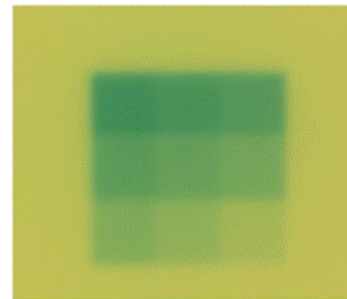

Not online information

Conventional ionization chambers



Recombination

Ultra-thin parallel ionization chamber^[1]



Prototype

Diamond detectors



Under research at UHDR

[1] F. Gómez et al. *Med. Phys.* 2022, 49: 4705

Online beam monitoring detector. FLASH irradiations

Requirements:

- Extended dynamic range
- High temporal resolution
- Radiation hardness

Organic plastic scintillators



Online beam monitoring detector. FLASH irradiations

Requirements:

- ✓ Extended dynamic range
- ✓ High temporal resolution
- ✓ Radiation hardness

Organic plastic scintillators



+

- ✓ Water equivalent
- ✓ Energy independent
- ✓ Dose and dose rate linearity
- ✓ Wide variety of geometries and sizes

Online beam monitoring detector. FLASH irradiations

Requirements:

- ✓ Extended dynamic range
- ✓ High temporal resolution
- ✓ Radiation hardness

+


- ✓ Water equivalent
- ✓ Energy independent
- ✓ Dose and dose rate linearity
- ✓ Wide variety of geometries and sizes

Organic plastic scintillators




**Perfect candidate
for an online
beam monitor
detector**

Detector proposed: Plastic scintillator coupled to a SiPM via an optical fiber

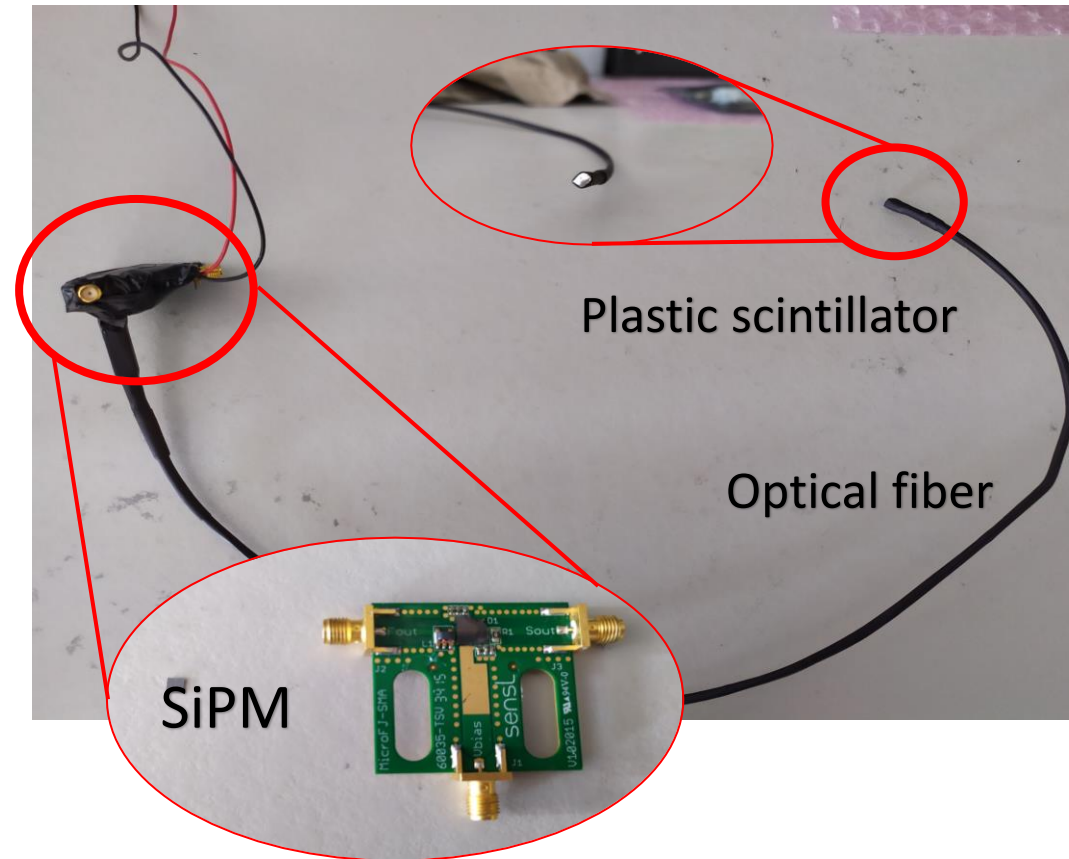

Scheme of the detector. It consists of a plastic scintillator (right) attached via an optical fiber to a SiPM (left).


Detector proposed: Plastic scintillator coupled to a SiPM via an optical fiber

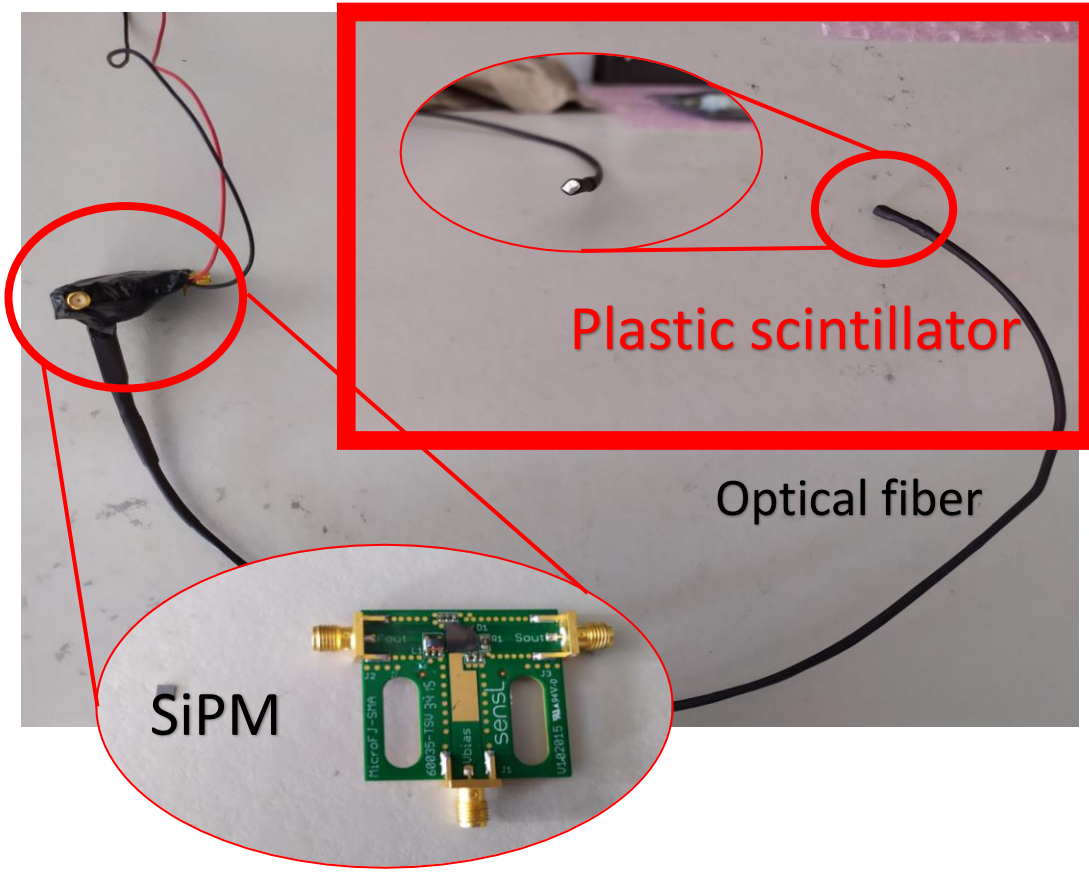

3 x 3 x 3 mm³ fast plastic scintillator
Eljen Technology EJ-232Q quenched
with 0.5% benzophenone



Detector proposed: Plastic scintillator coupled to a SiPM via an optical fiber

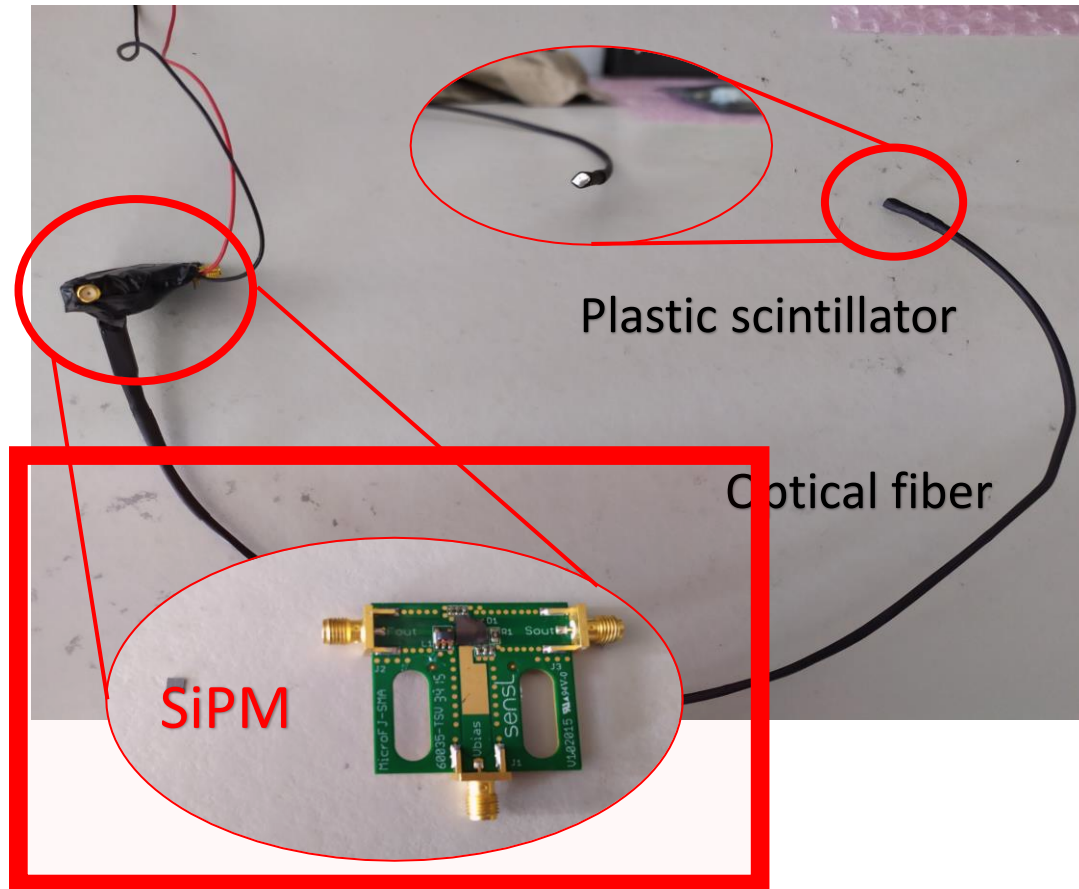

3 x 3 mm² SiPM


MicroFJ-SMA-30035, Onsemi (former sensL)

Biased at 28 V (Tenma 72-2550)

Mounted on a PCB board (MicroFJ-SMA-30035-GEVB, Onsemi)



Detector proposed: Plastic scintillator coupled to a SiPM via an optical fiber

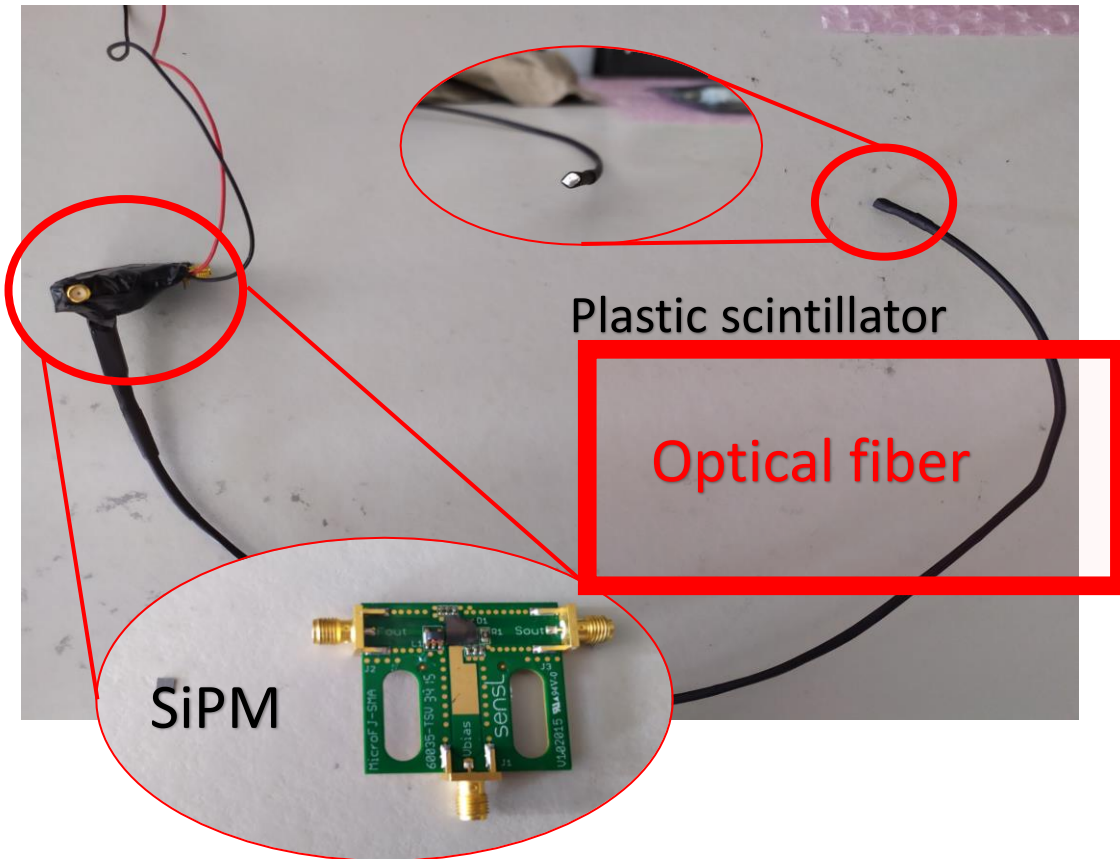

Optical fiber



Assembly of 10 optical fibers.

Diameter 0.8 mm each

Length: 63 cm


Norland Optical Adhesive 61 applied between the optical fibers, SiPM and plastic.

Detector proposed: Plastic scintillator coupled to a SiPM via an optical fiber

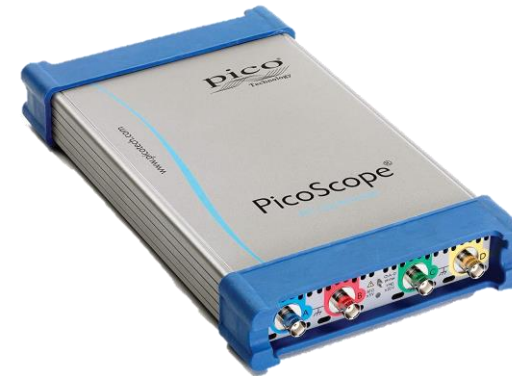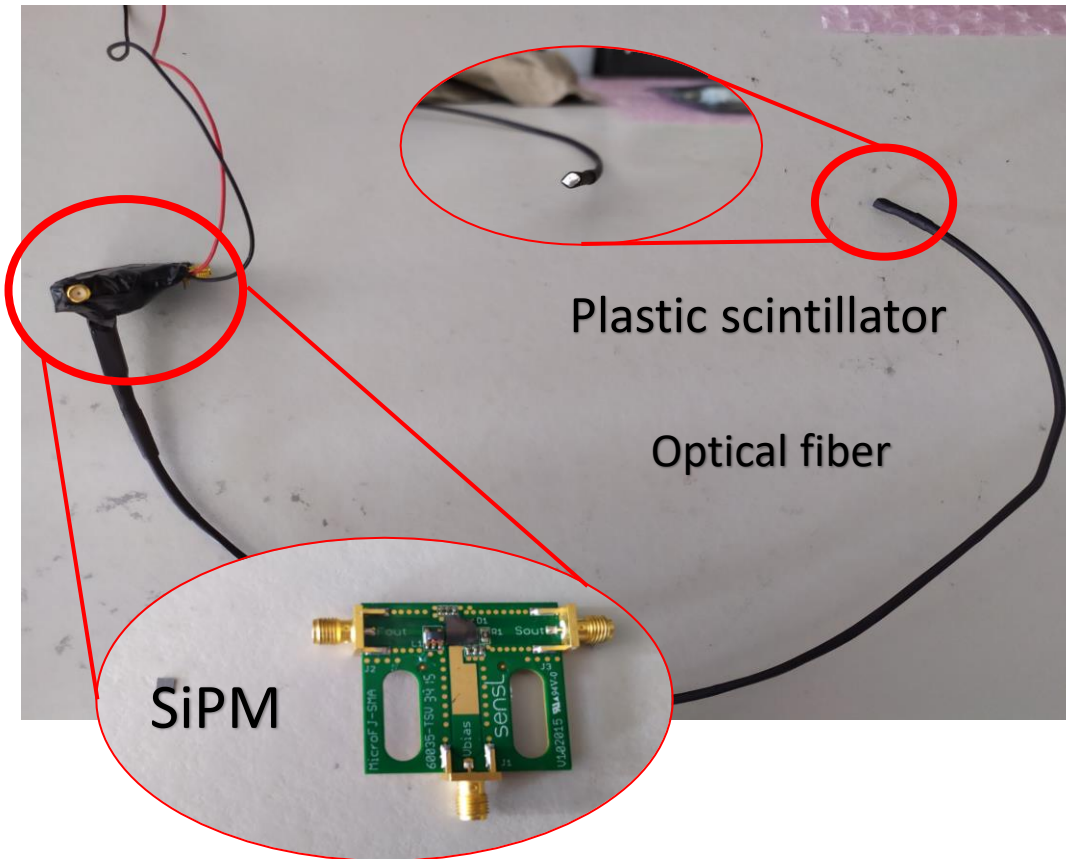

Processing board
(Picoscope 6403D)
8-bit digital scope
Bandwidth 350 MHz
Sampling rate 5GS/s

Objective

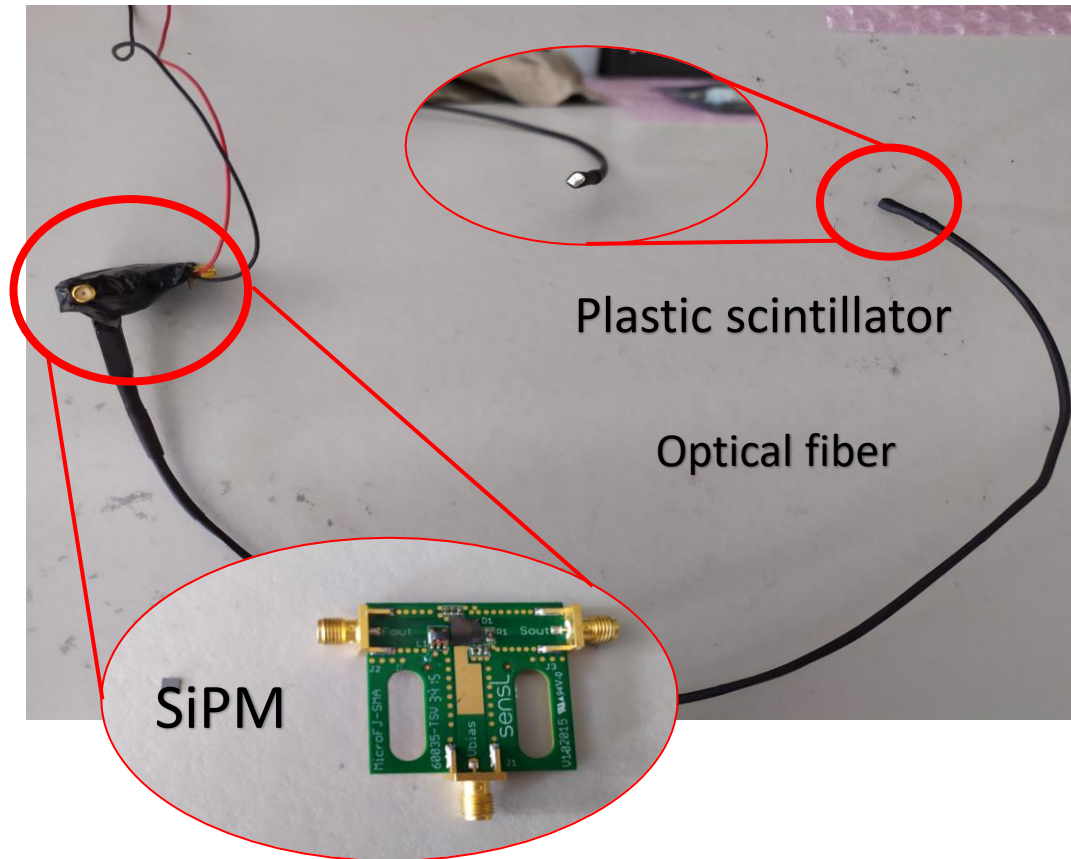

Evaluation of the **timing capabilities** of a novel plastic scintillator fiber optic detector coupled to a SiPM and read out by an ultrafast data acquisition system in a clinical proton beam.


Quironsalud Protontherapy Center (Madrid)

IBA Proteus-One

Synchrocyclotron S2C2, RF 60-90 MHz
Proton energies: 70-230 MeV
Pulse repetition rate: 1000 μ s
Pulse width: 10 μ s



Quironsalud Protontherapy Center (Madrid)

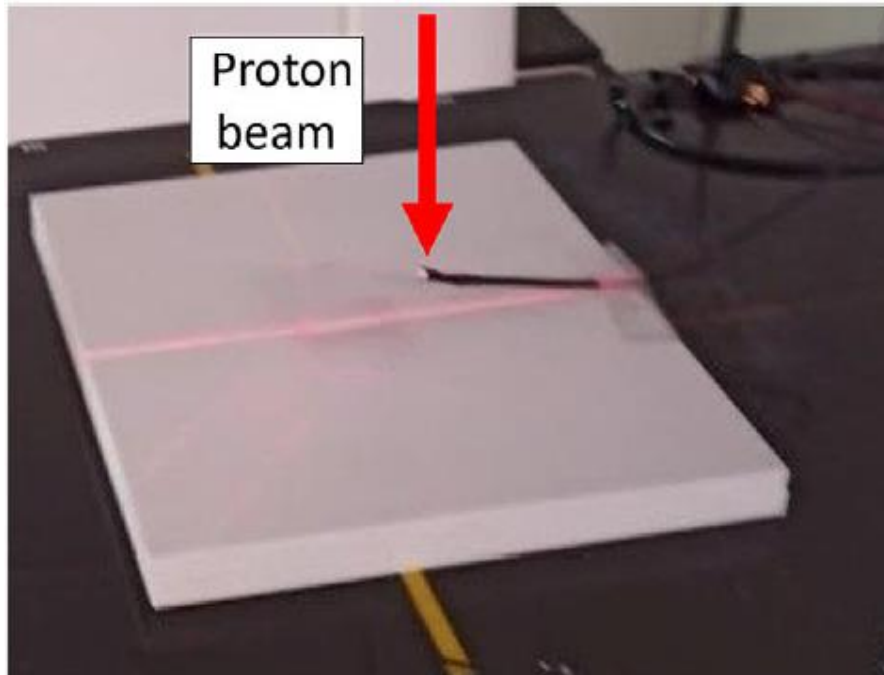

Irradiation conditions:

70 MeV proton beam

8 mm² sigma spot size

Beam current: 8.98 nA


Detector perpendicular to the beam

Irradiations at the isocenter

Two recording lengths:


- Sampling rate of 4.76 MS/s (210 ns in between samples)
- Sampling rate of 1.25GS/s (0.8 ns in between samples)

Characteristic pulse structure. 10 ms region

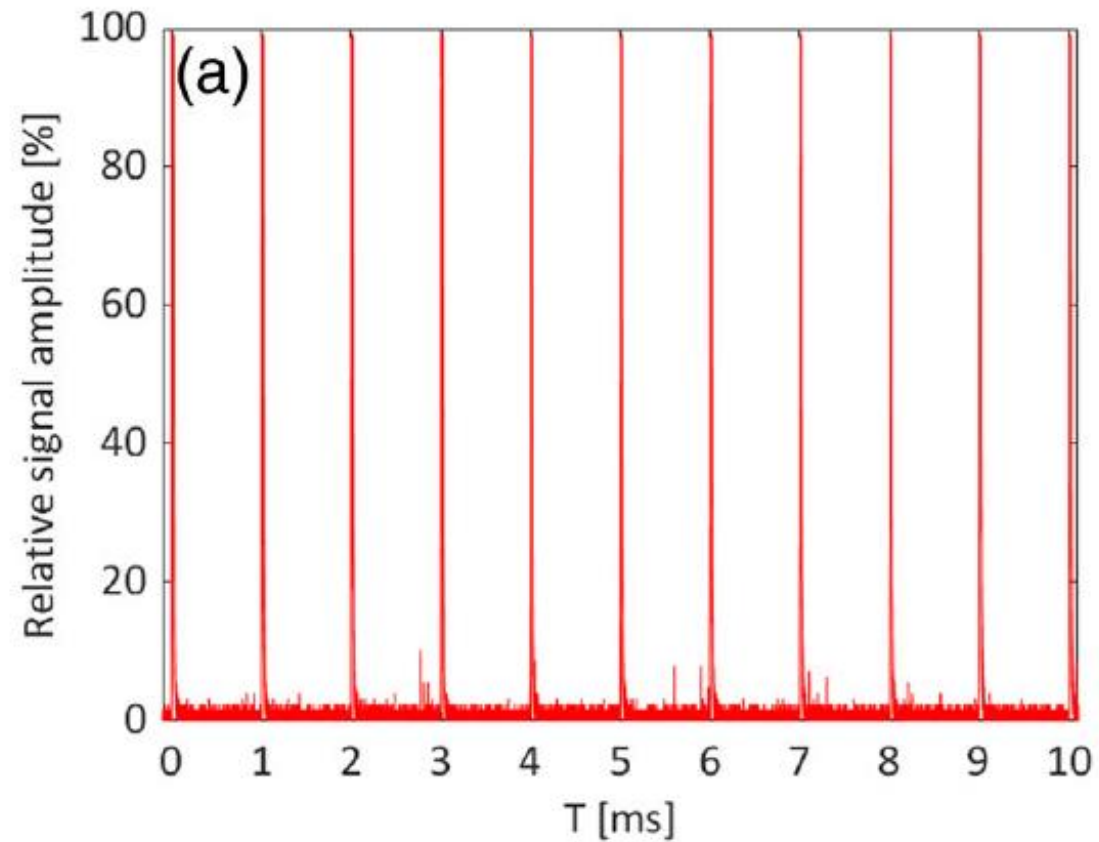


- Signal intensity for a sequence of 10 spots
- 1 ms repetition rate.
- 10 μ s width macro-pulses
- Sampling period 210 ns

Individual measurement of a single pulse

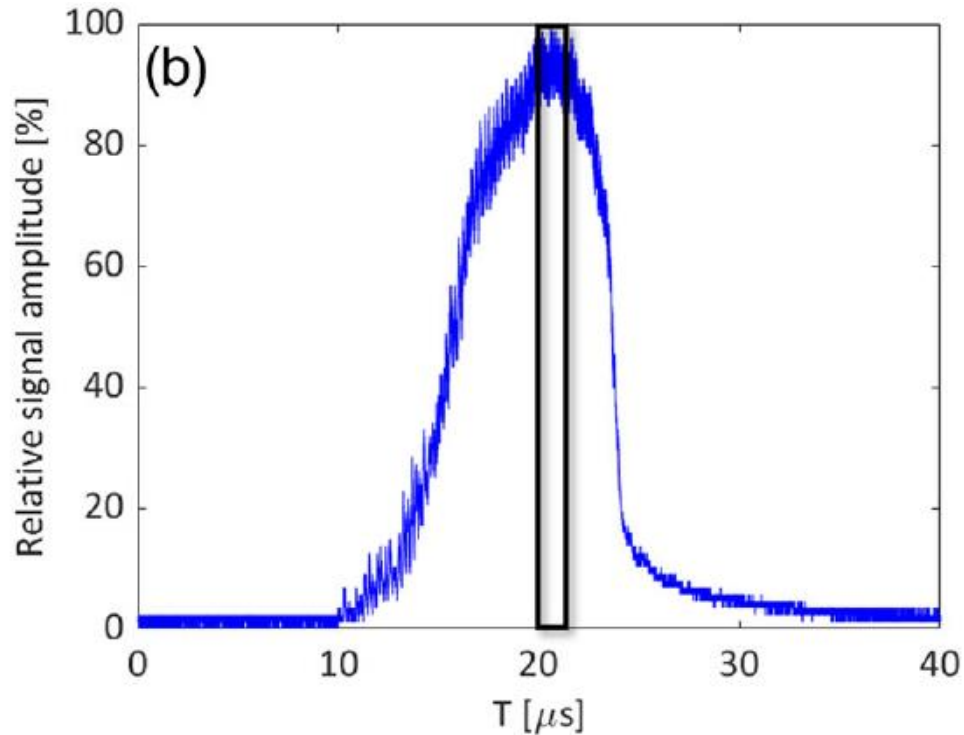


200 ns zoom. Micro-bunch

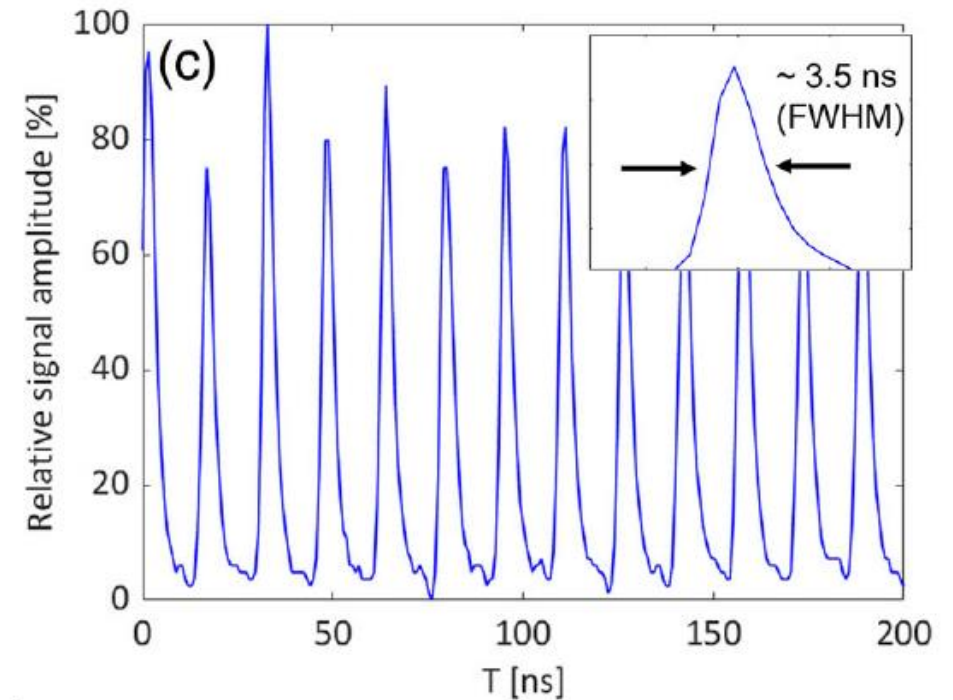

- Characteristic width of 10 μs
- Ripples are observed due to the accelerator RF system

- Micro-bunch period of 16 ns
- FWHM of about 3.5 ns.

Frequency spectra

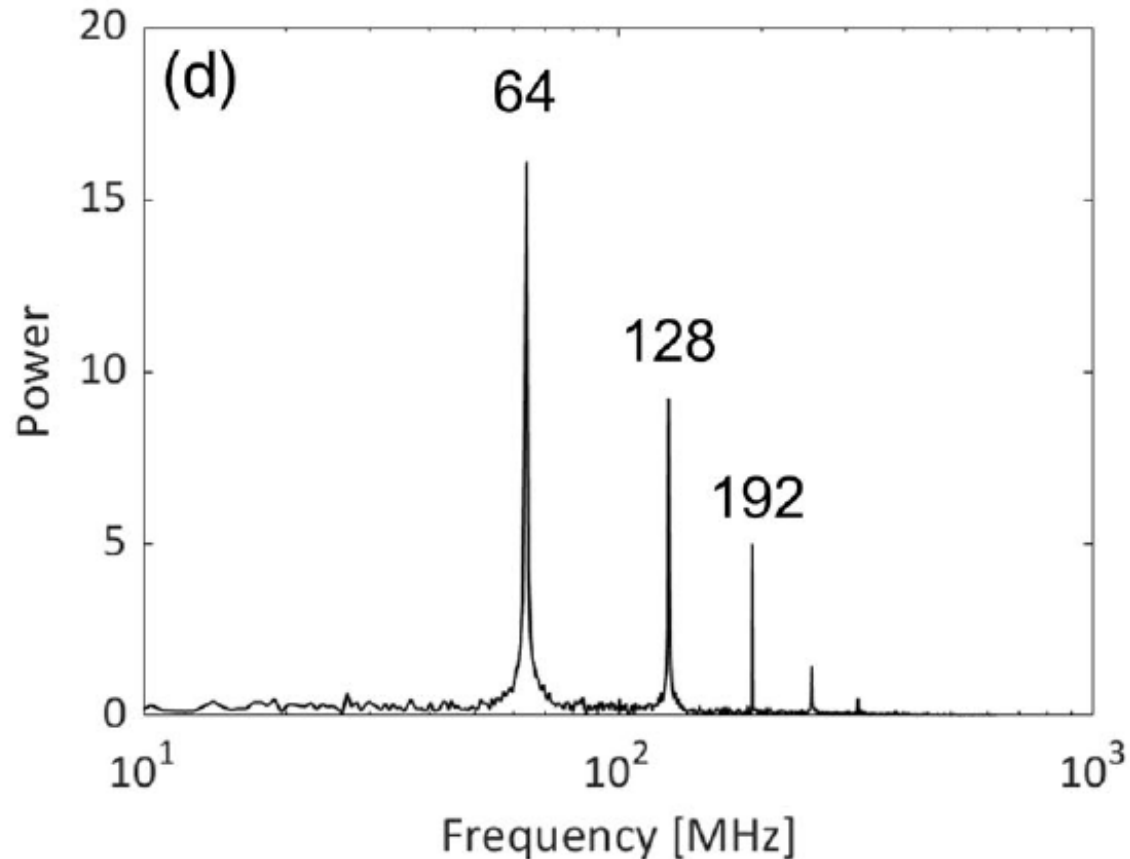

- Fast Fourier Transform (FFT) spectrum analyzer tool in MATLAB (R2021b).
- Analysis of 2048 samples ($\sim 1.6 \mu\text{s}$)
- Sampling period 0.8 ns
- Good agreement with the synchrocyclotron frequency

Each pulse presents a sub- μs structure, with a characteristic frequency of 64 MHz, measured with a sampling period of 0.8 ns

The proposed system was able to measure the fine time structure of a clinical proton accelerator online and with sub-ns time resolution.

Received: 6 October 2022 | Revised: 27 January 2023 | Accepted: 20 February 2023

DOI: 10.1002/mp.16333

What's

TECHNICAL NOTE

MEDICAL PHYSICS

Technical note: Measurement of the bunch structure of a clinical proton beam using a SiPM coupled to a plastic scintillator with an optical fiber

Miguel García Díez^{1,2}  | Andrea Espinosa Rodriguez^{1,2}  |
Victor Sánchez Tembleque^{1,2}  | Daniel Sánchez Parcerisa^{1,2}  |
Victor Valladolid Onecha^{1,2} | Juan A. Vera Sanchez³  | Alejandro Mazal³  |
Luis Mario Fraile^{1,2}  | Jose Manuel Udias^{1,2} 

¹Grupo de Física Nuclear, EMFTEL & IPARCOS, Universidad Complutense de Madrid, CEI Moncloa, Madrid, Spain

Abstract

Background: Recent proposals of high dose rate plans in protontherapy as well as very short proton bunches may pose problems to current beam monitor

The proposed system was able to measure the fine time structure of a clinical proton accelerator online and with sub-ns time resolution.

What's next?

- **Other combination of SiPM + optic fiber**

Time resolution (FWHM) for different SiPM + plastic scintillator measured from coincidences for 511 keV gamma photons from a ^{22}Na source

This work

Next work

SiPM	Fiber	Length (cm)	Time resolution (ps)
S13360-3075CS	Plastic coupled directly		58 (10)
MicroFJ-SMA-30035	Plastic coupled directly		128 (4)
S13360-3075CS	Set of fibers	60	638 (5)
MicroFJ-SMA-30035	Set of fibers	60	715 (5)
S13360-3075CS	Solid	10	176 (4)
S13360-3075CS	Solid	60	329 (5)

The proposed system was able to measure the fine time structure of a clinical proton accelerator online and with sub-ns time resolution.


What's next?

- Other combination of SiPM + optic fiber
- **Study potential to measure absolute dose**

The proposed system was able to measure the fine time structure of a clinical proton accelerator online and with sub-ns time resolution.

What's next?

- Other combination of SiPM + optic fiber
- Study potential to measure absolute dose
- Incorporate the detector in a FLASH X-ray based preclinical irradiator

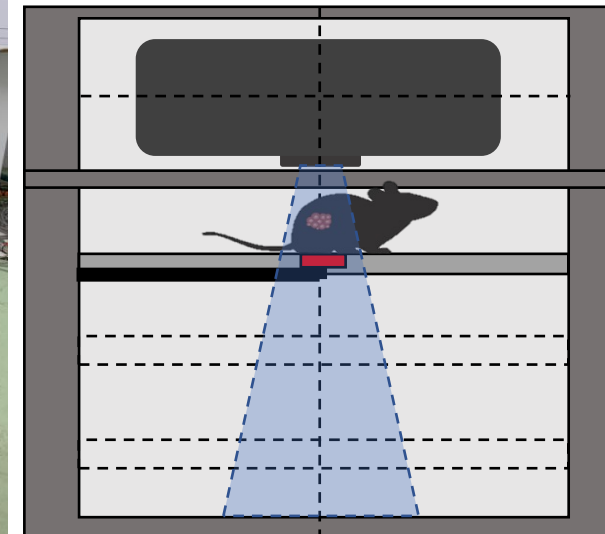

Thank you for your attention!

Espinosa-Rodriguez, *Radiat. Phys. Chem.*, 2023 110760.

Online beam monitoring detector for FLASH irradiations



Paula Ibáñez García

Grupo de Física Nuclear & IPARCOS, Universidad
Complutense de Madrid

Instituto de Investigación Sanitaria del Hospital Clínico San
Carlos

Miguel García Díez, Andrea Espinosa, Víctor Sánchez -Tembleque, Daniel
Sánchez-Parcerisa, Víctor Valladolid, Juan A. Vera, Alejandro Mazal, Luis Mario
Fraile, José Manuel Udías