



Part E. Radiation monitors

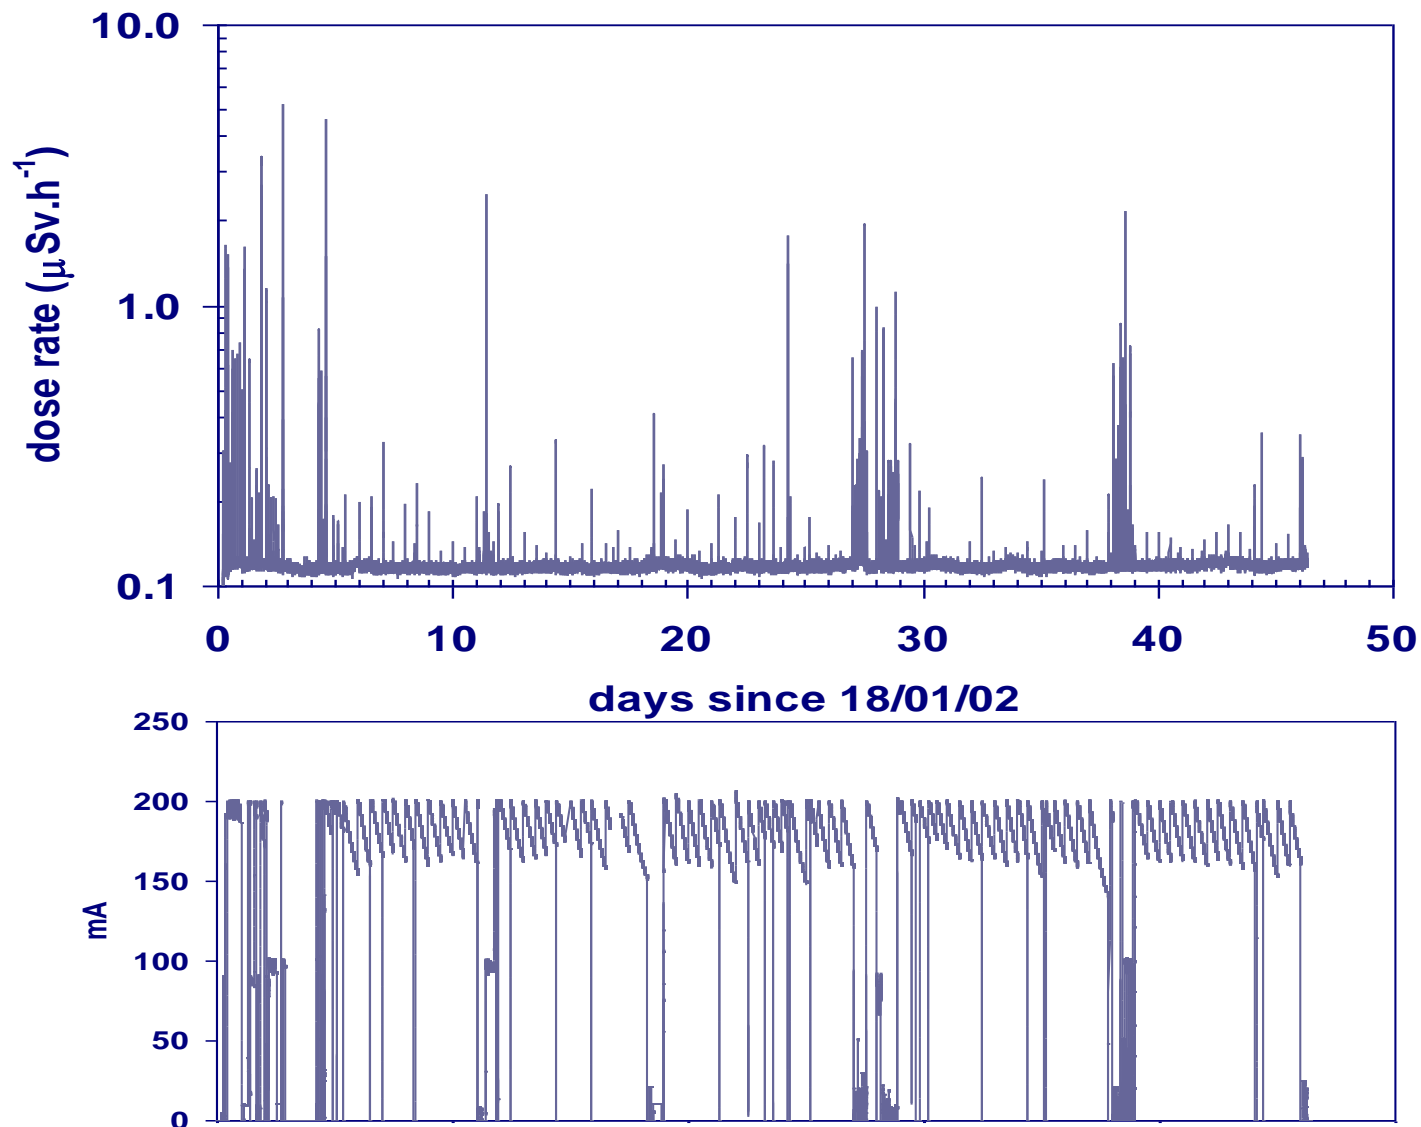

Example: photon dose rate measurement around ESRF storage ring

Gas-filled detectors

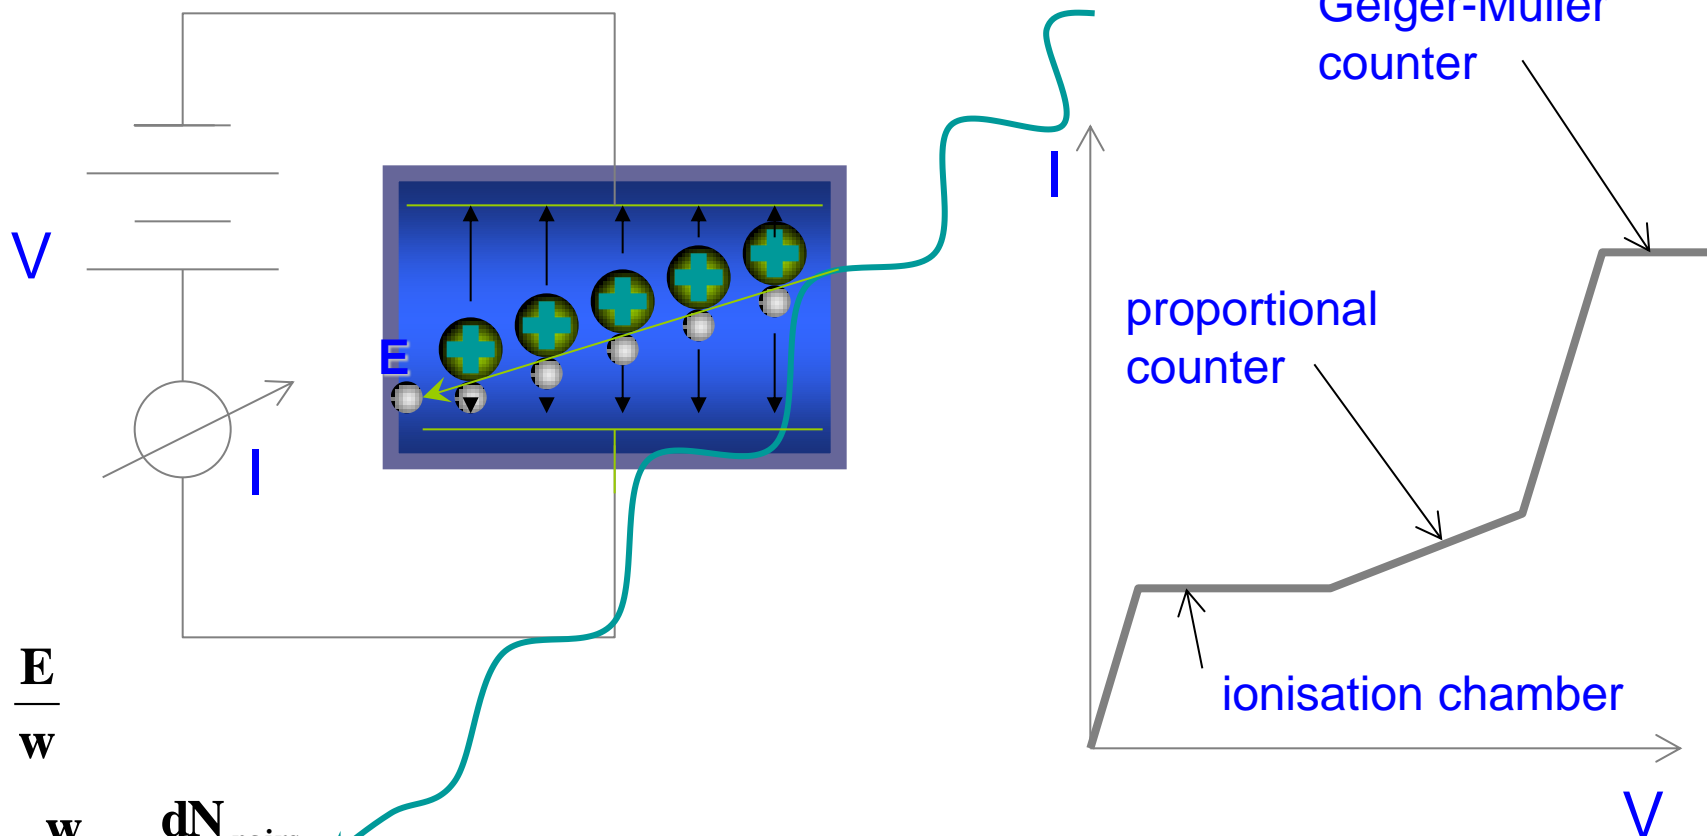


$$N_{\text{pairs}} = \frac{E}{w}$$

$$\frac{dD}{dt} \propto \frac{w}{\rho_{\text{gas}} V_{\text{gas}}} \frac{dN_{\text{pairs}}}{dt}$$

$$\frac{dD}{dt} \propto \frac{w}{e \rho_{\text{gas}} V_{\text{gas}}} I$$

w	H ₂	He	O ₂	Ar	Air
electrons	36.3 eV	41 eV	31 eV	26.4 eV	34 eV
alphas	36.5 eV	44 eV	32.4 eV	26.4 eV	35.3 eV

Ionization chambers

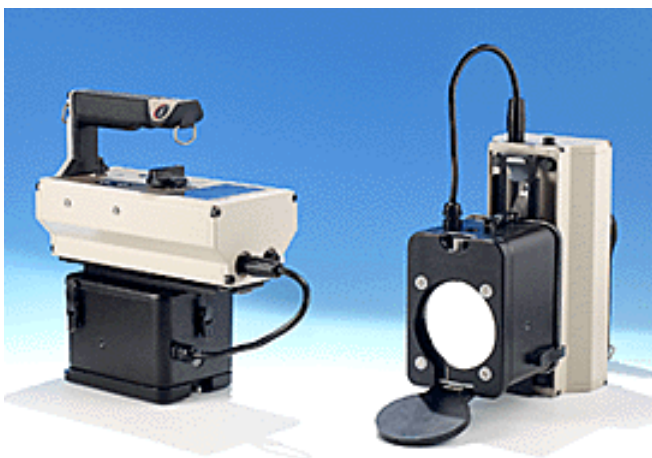


Proportional counter



Geiger - Müller counter







Neutron monitors

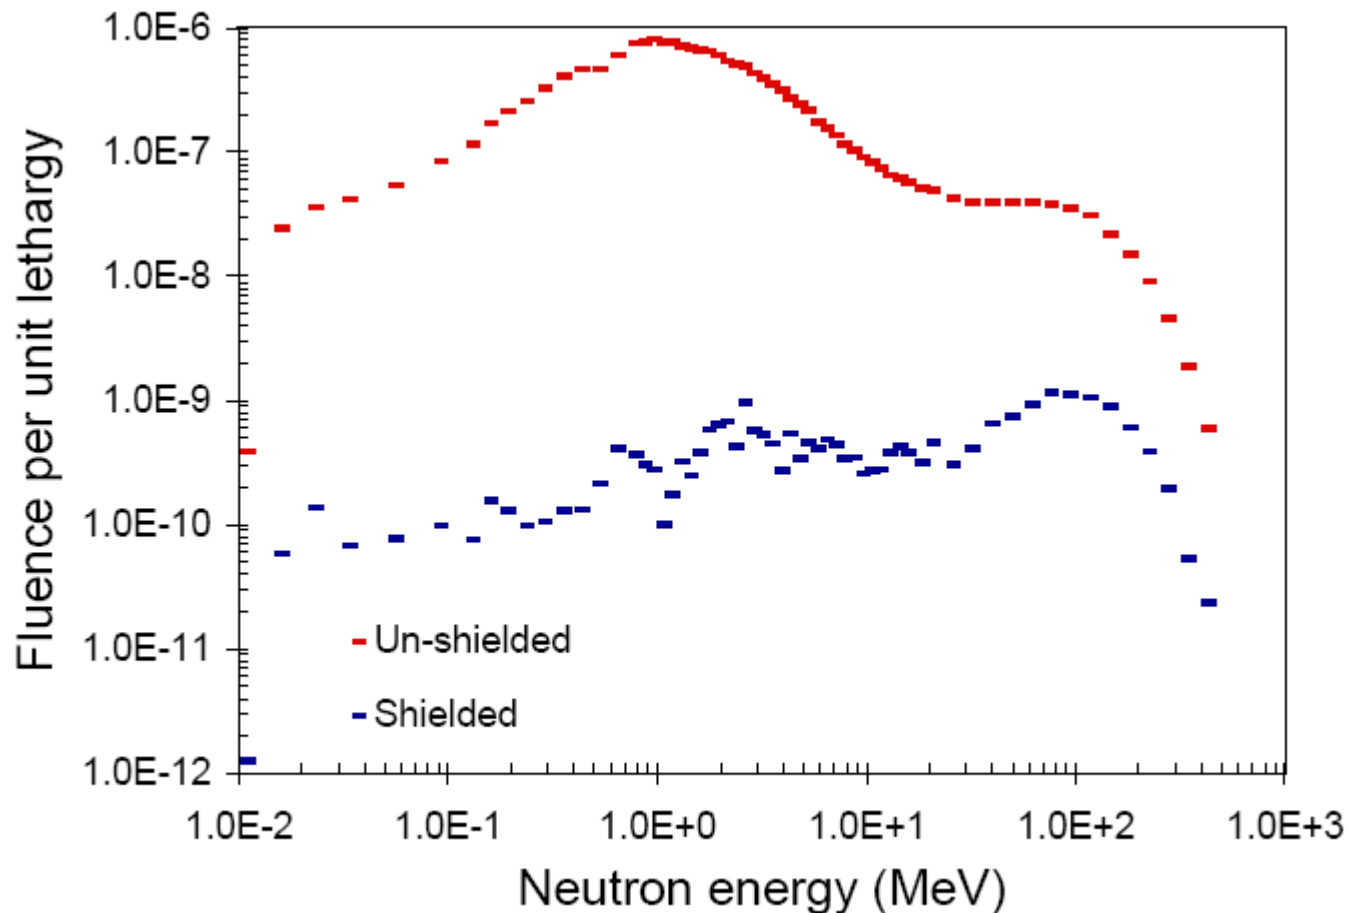


Example: neutron spectrum around the 1.7 GeV BESSY storage ring (Courtesy of Klaus Ott)

Moderated neutron monitors

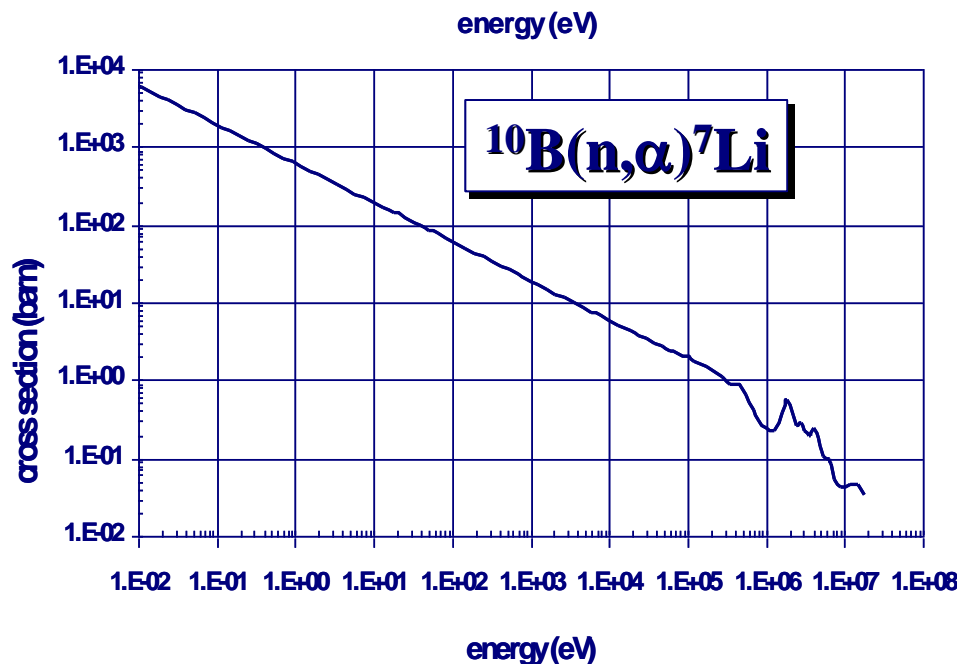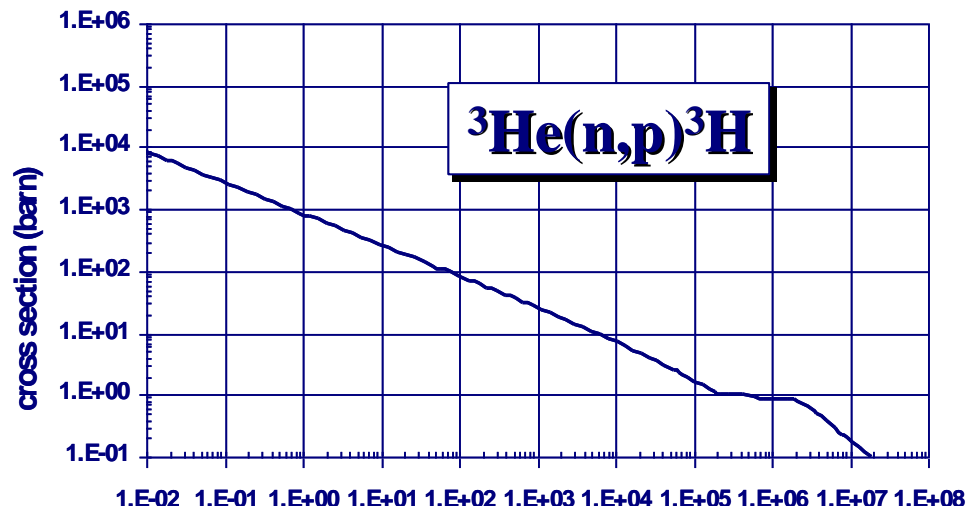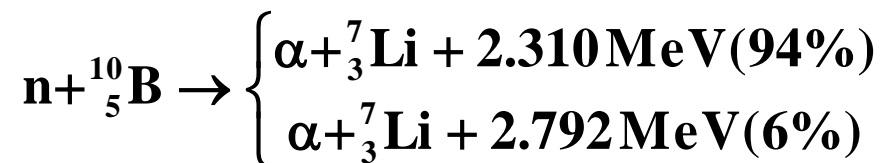³He-filled proportional counter:BF₃ counter:

→ Polyethylene moderator





Moderated neutron monitors

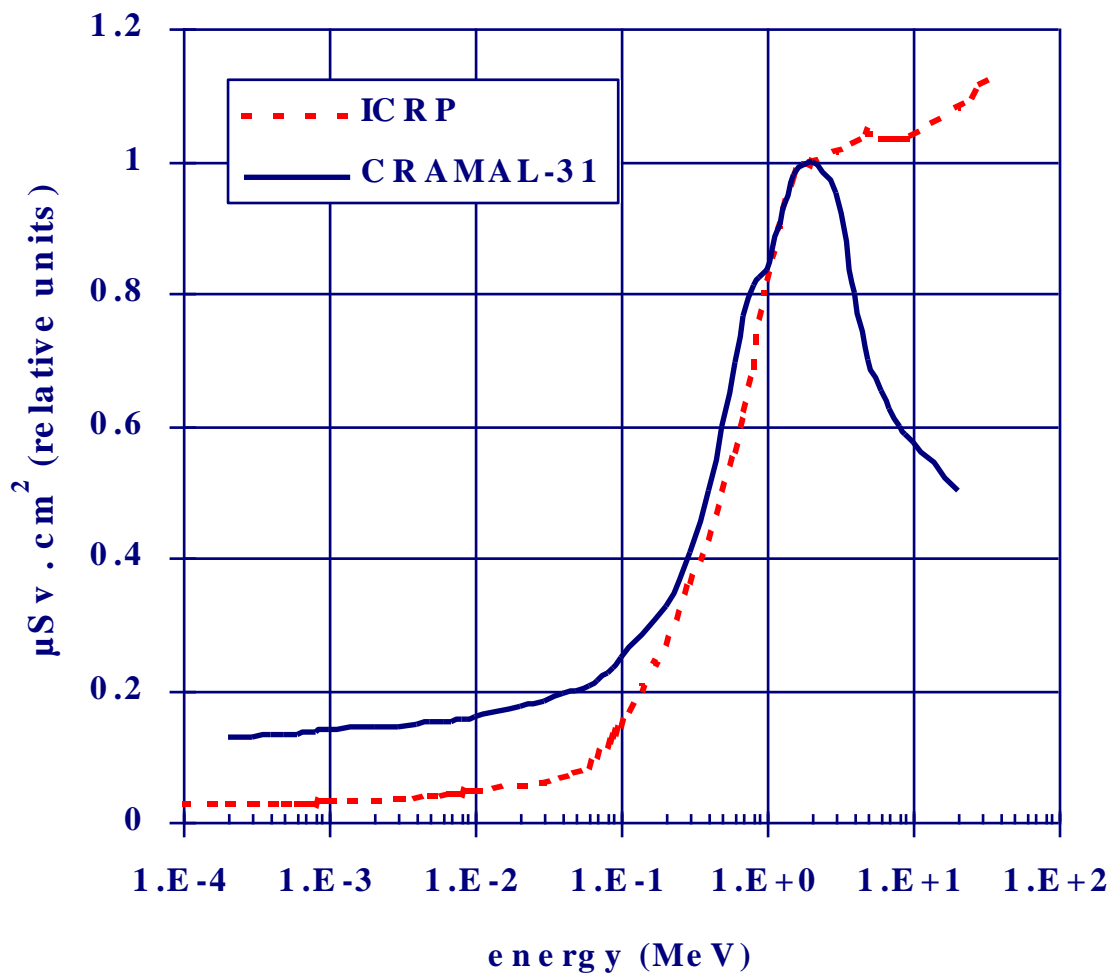

Moderated neutron monitors





Berthold
LB-6411

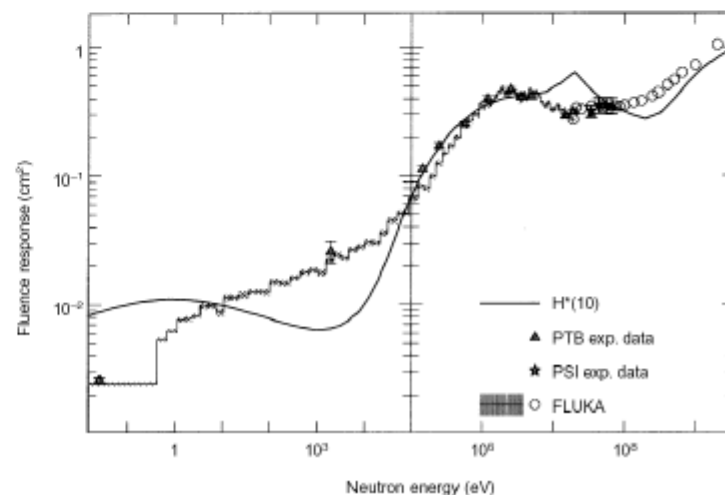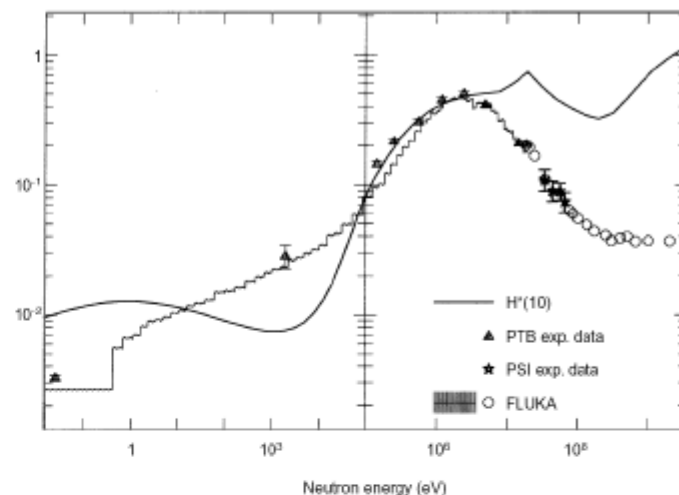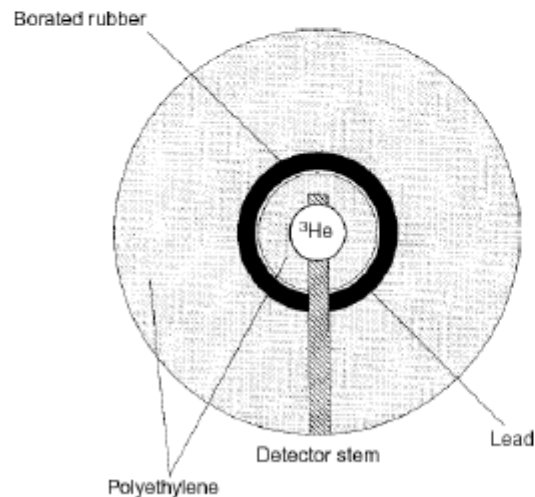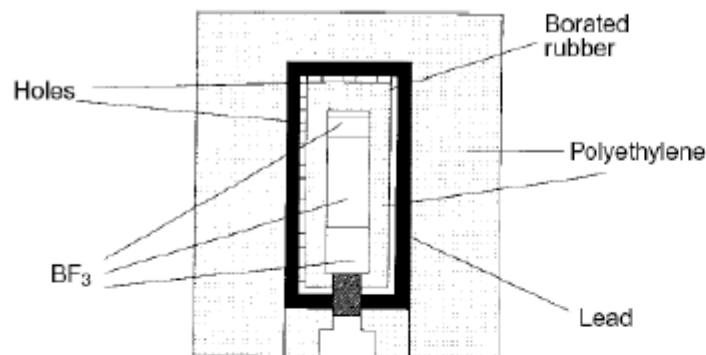


Neutron response enhancement using lead-shell in moderator type counters

Superheated emulsions

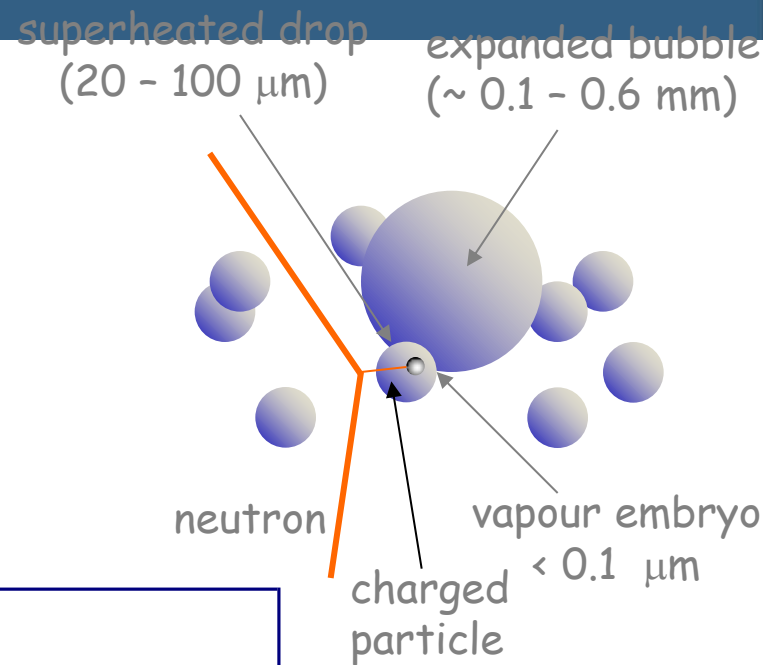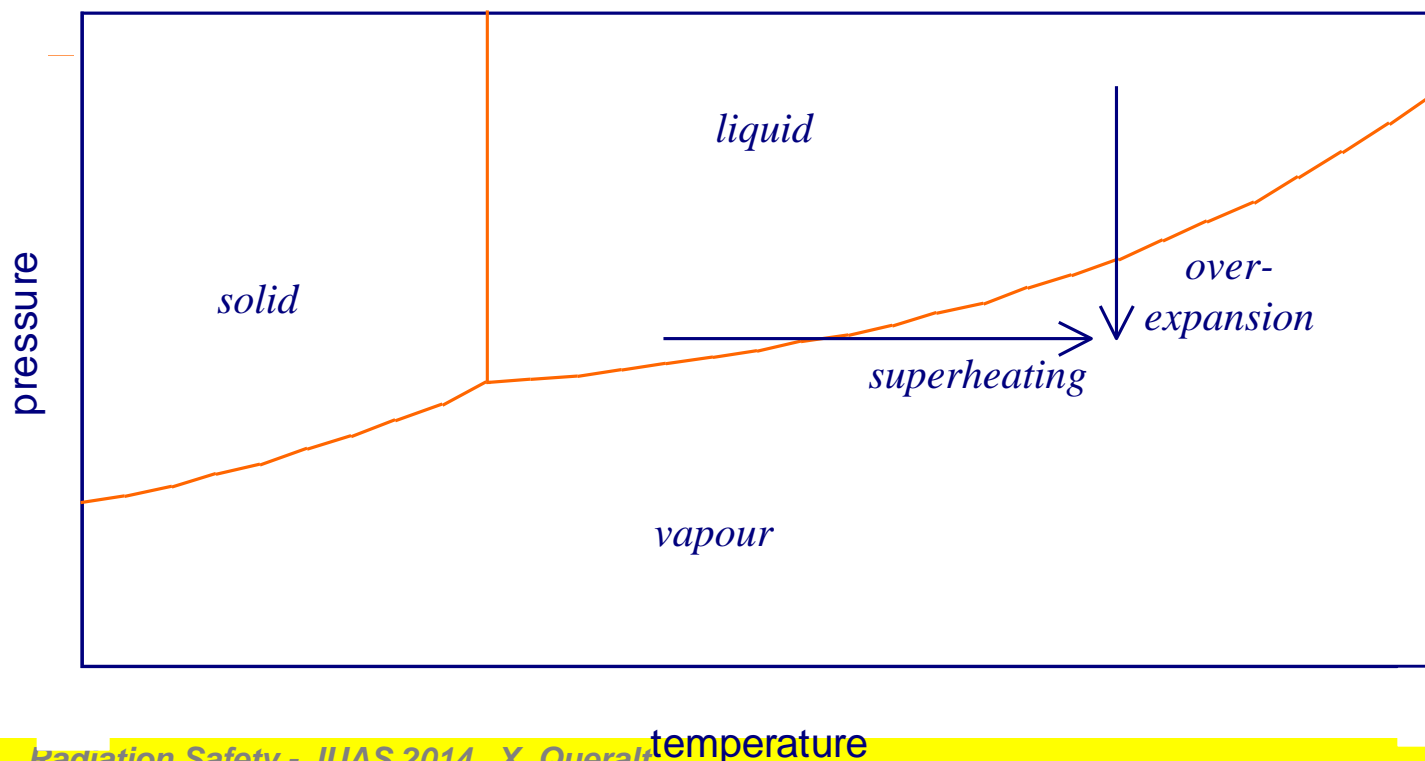

Superheated emulsions

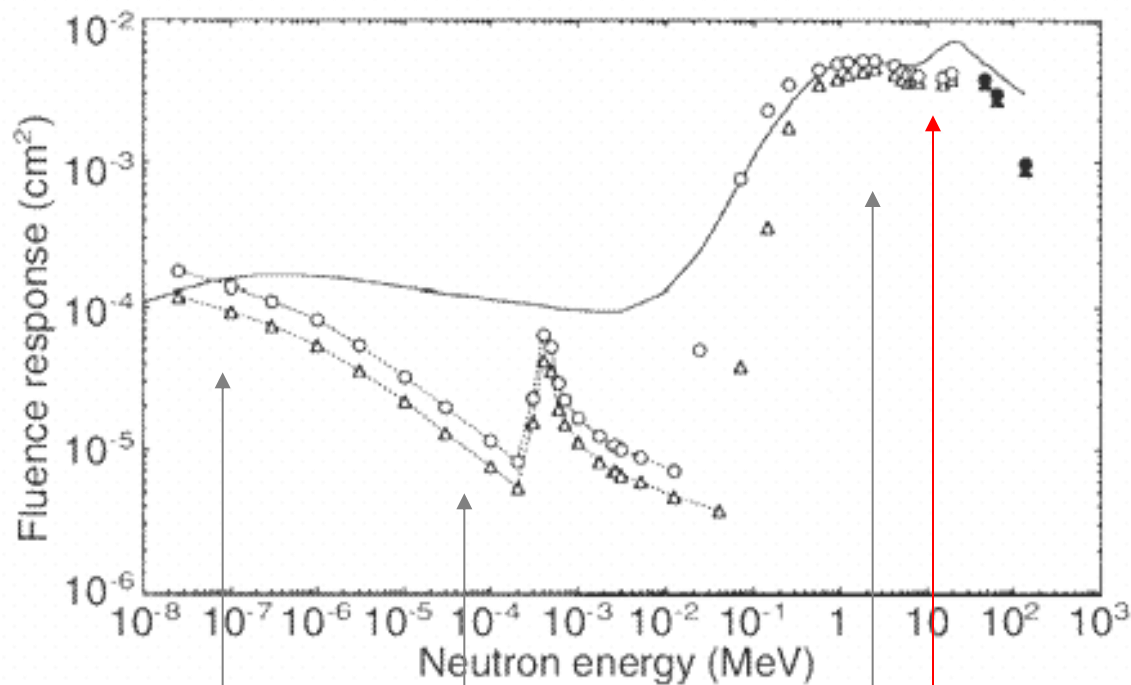

Thermal neutrons: OK


0.1 – 10 MeV: OK

Epithermal neutrons: not important

Under-read > 10 MeV



Energy response of SDD100 vials (dichlorodifluoromethane)

Superheated emulsions

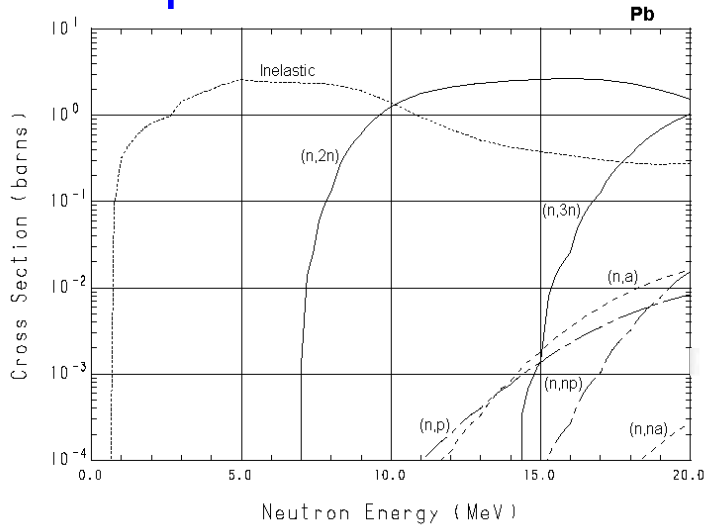


effect of lead moderator

ABC-HE with lead-shell



MCNPX simulation geometry


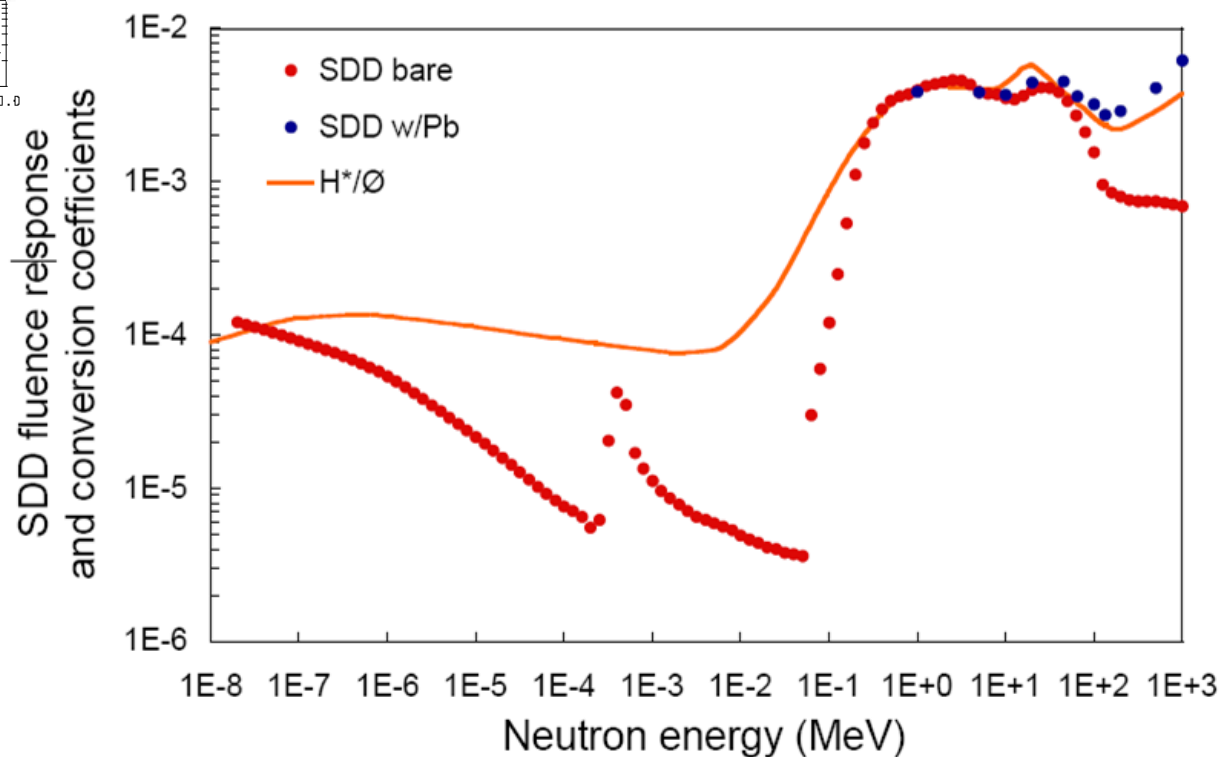


Superheated emulsions

Acoustic bubble counting

Model ABC1260

Framework Scientific

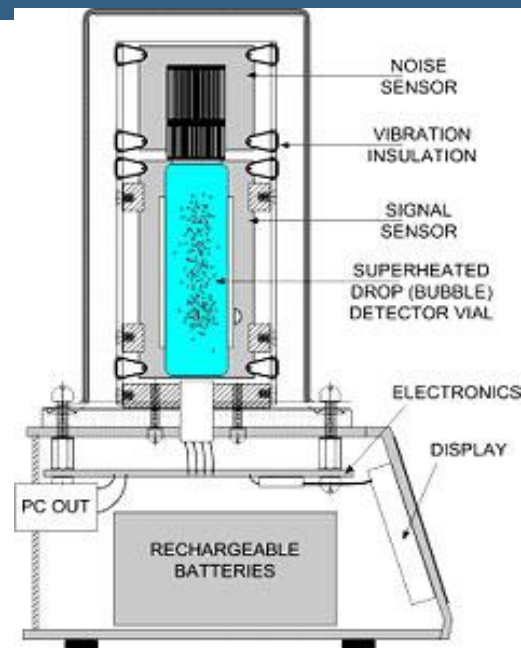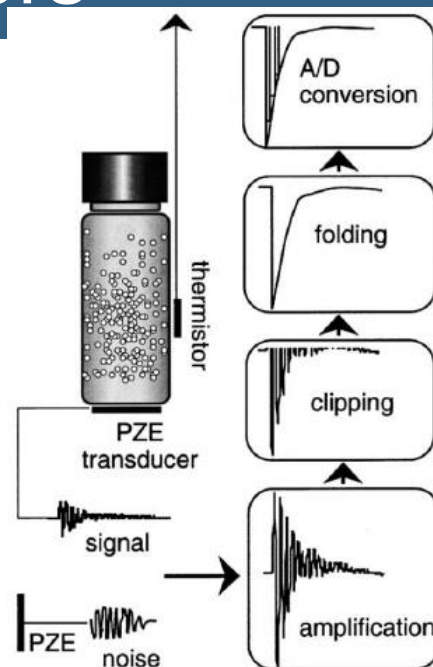www.framesci.com




Gamma (X-ray)

Gamma (X-ray)

Spectrometer



Gamma (X-ray)

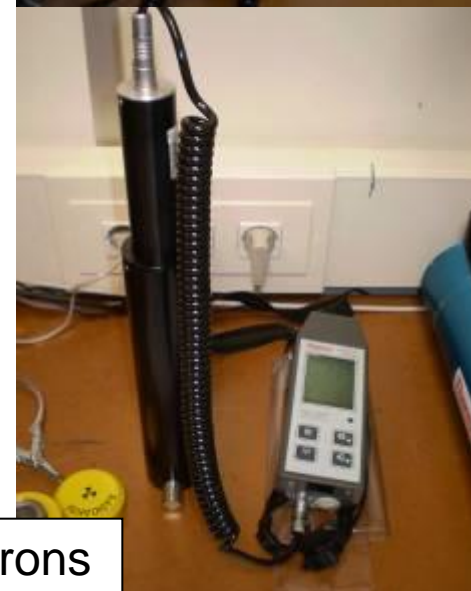

Neutrons

COMPANY	MODEL	ENERGY RANGE	DETECTION RANGE
THERMO	SmartION Mini 2100S	>10keV	0-500mSv/h
FLUKE	Victoreen 451P	>25keV	<50mSv/h
THERMO	FH40 G-L10	>30keV	10nSv/h - 100mSv/h
THERMO	FHZ 672 E-10:	48 keV - 4.4 MeV	1nSv/h - 100mSv/h
THERMO	RadEye PRD	30 keV – 1.3 MeV	0.01 μ Sv/h – 250 μ Sv/h
THERMO	FHT 752 SH		0.01 - 100,000 cps
THERMO	RadEye N		>0.005 cps

- Active radiation detectors:

	FHT192	FHT 762 Wendi-2	EPD
0 Manufacturer	Thermo Electron GmbH	Thermo Electron GmbH	Thermo Electron GmbH
1 Particle	Photons	Neutrons	Photons
2 Energy range	30 keV– 7 MeV	25 meV–5 GeV	15 keV–10 MeV
3 Measuring range	100 nSv/h–1 Sv/h	1 nSv/h – 100 mSv/h	Resol. 1 mSv/h: <0.5 Sv/h – 4 Sv/h Resol. 1 Sv/h: 4–50 Sv/h
4 Energy response	Calibration factor resp. Cs-137: For low dose rate: 0.01-0.02 (μSv/h)/cps For high dose rate: 1.9 - 2.2 (μSv/h)/cps	Calibration Factor: 1.14 (μSv/h)/cps	Ref. Cs-137 ±30% from 17keV to 6MeV ±50% from 6MeV to 15Mev
5 Quantity	Hp(10)	Hp(10)	Hp(10)
8 Type	Active Ionization chamber	Active Proportional counter	Active semiconductor dosimeter
9 Sensitive material	Inert gas (7 bar)	He-3 (2 bar) + polyethylene moderator	Silicon diode detectors
10 Dead Time	Dead Time for high dose rate: 6-7 μs	Dead Time: 1.8 μs	--

➤ TR01GN: Tunnel Detector – Septum Magnet & Kickers




➤ TR01GN: Tunnel Detector – Septum Magnet & Kickers



1. Engineering solution


- Radiation Monitors Network reinforced by movables monitors

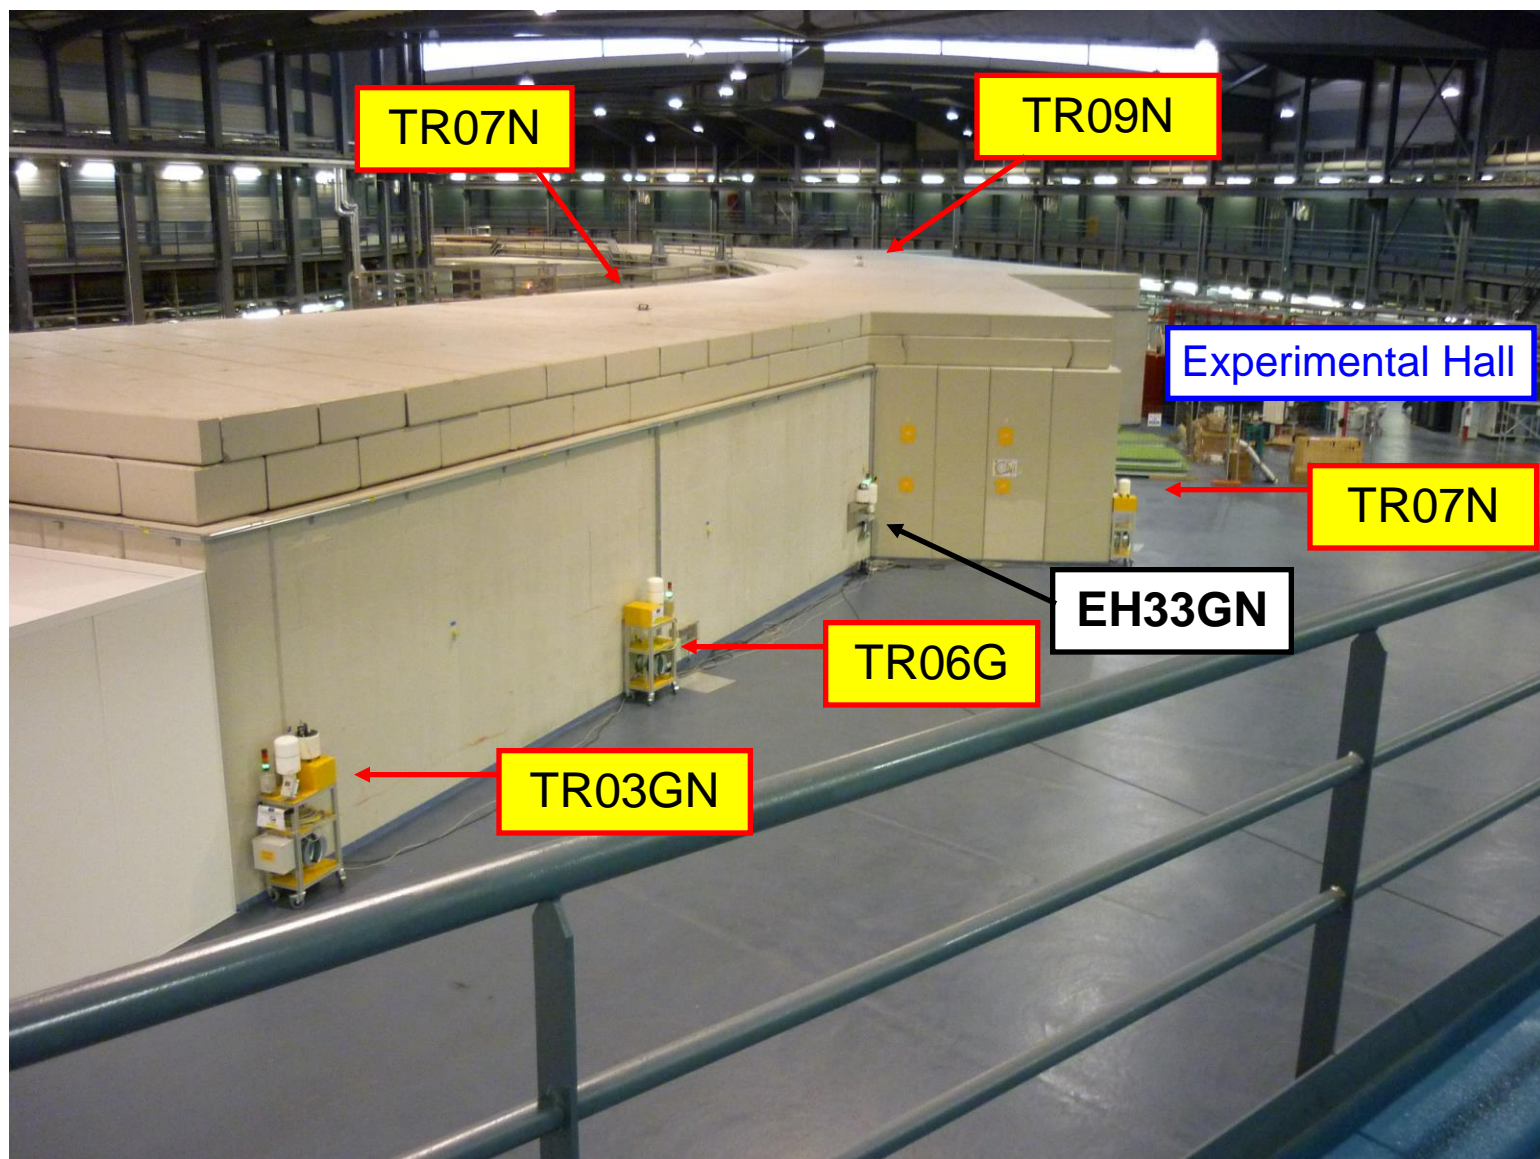

1. Engineering solution

September 16th '09


D2 Gamma DR (uSv/h)

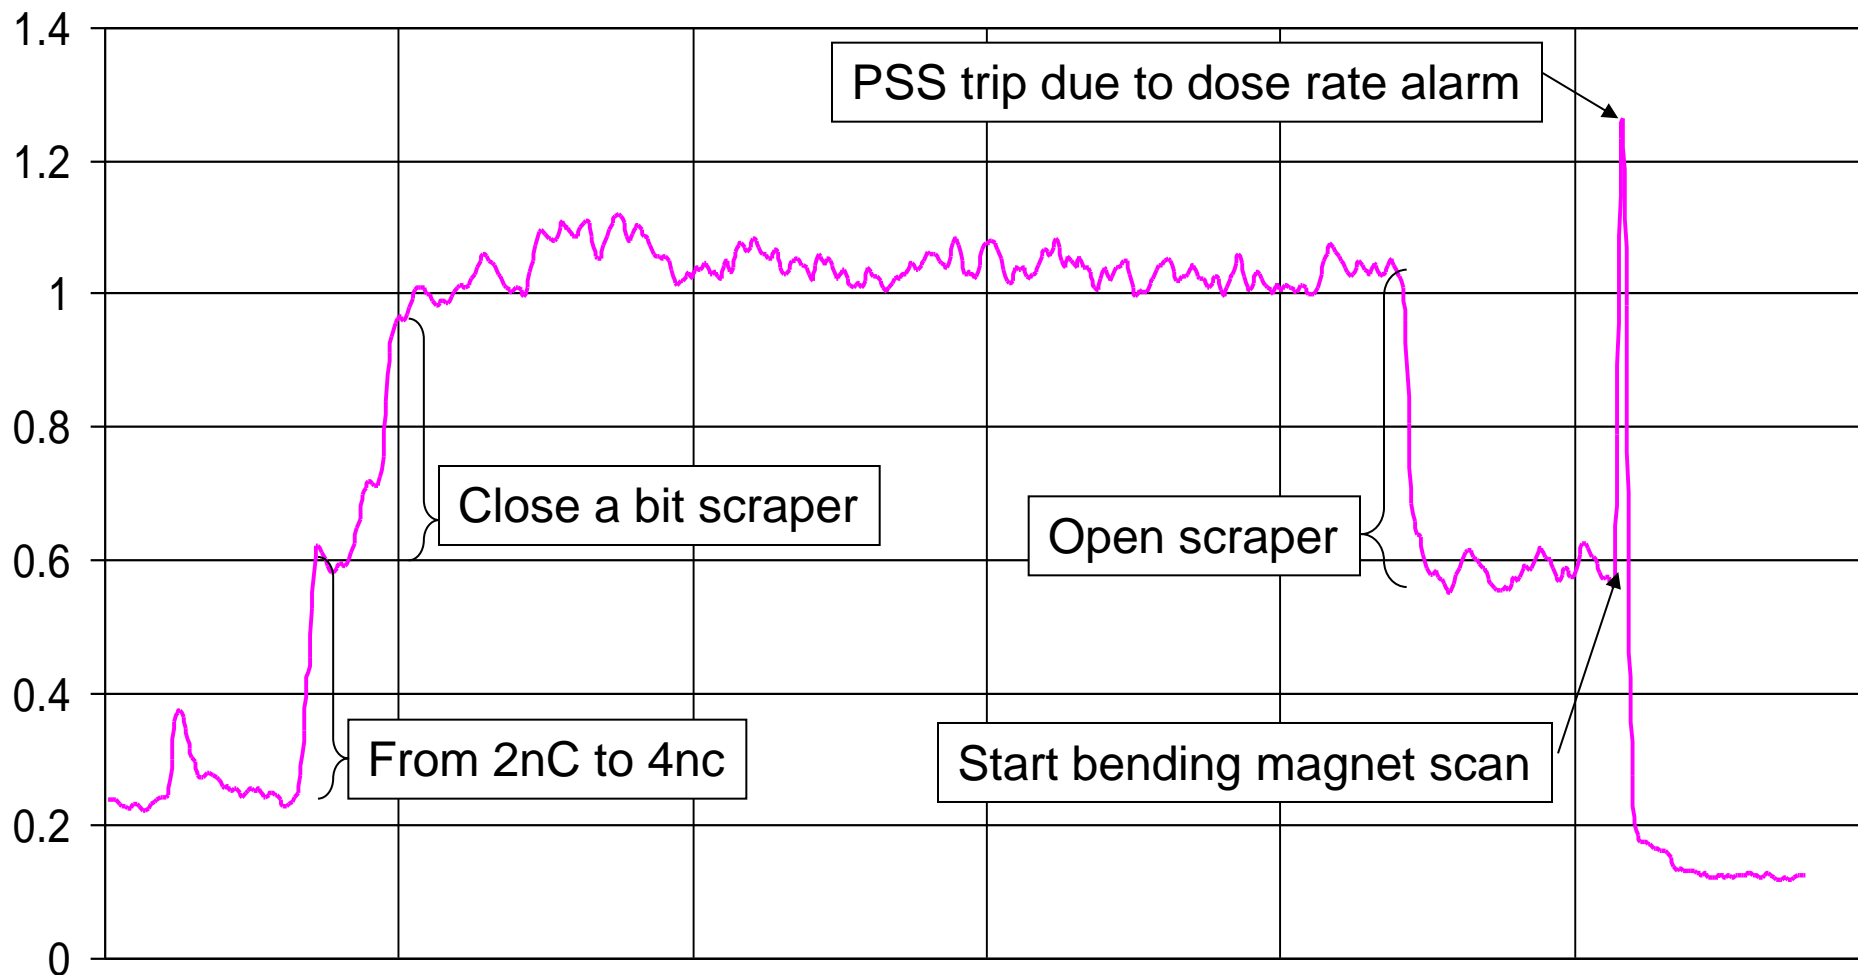

1. Engineering solution

RMN: Cu SCRAPPER DATA


Gamma dose rate due to the Cu scrapper scans

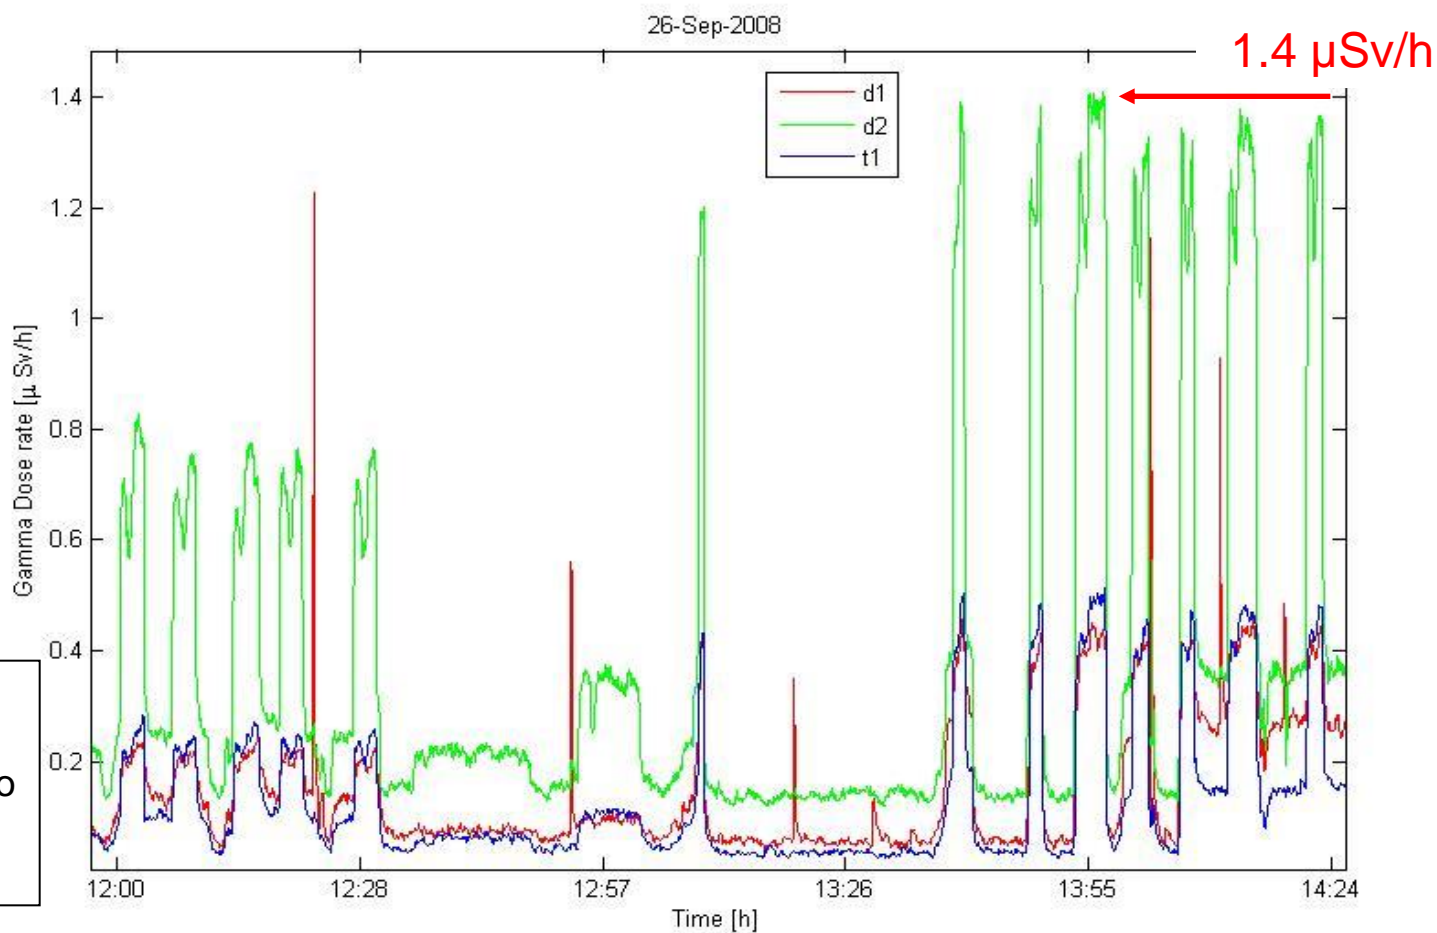

26-Sep-2008
SCRAPER SCANS
Charge/pulse: 4nC/pulso
Energy: 109MeV
Frequency: 1Hz


1. Engineering solution

RMN: LOCAL SHIELDING EFFECT

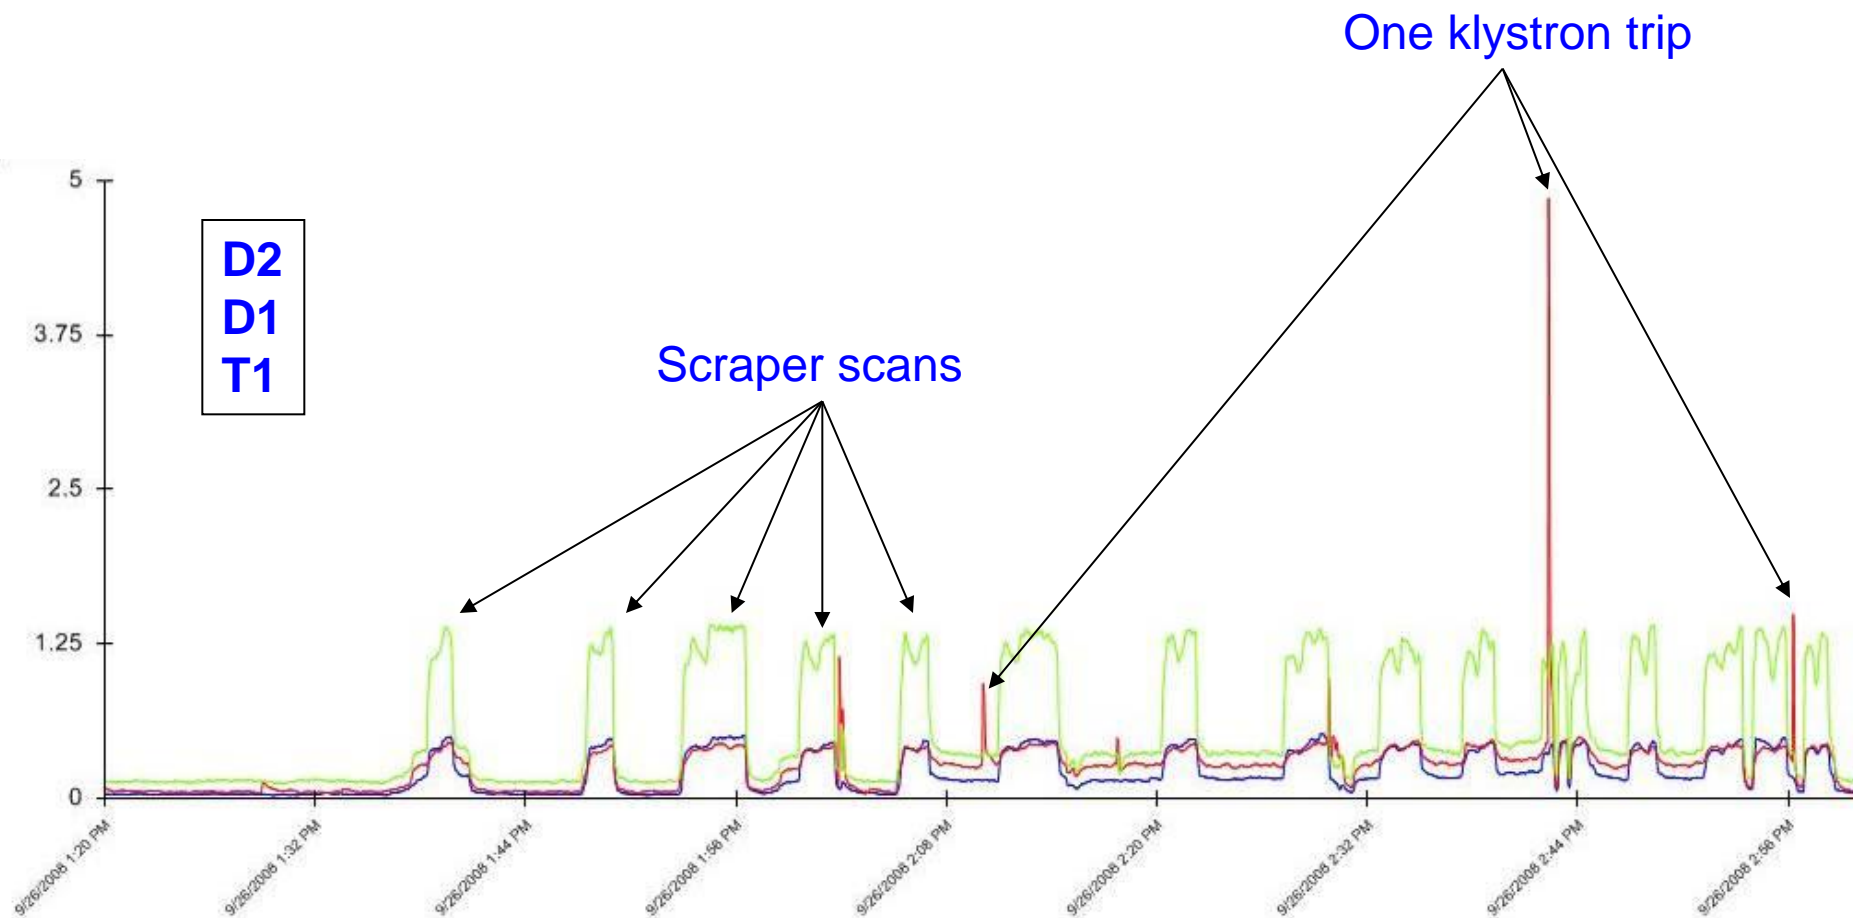


1. Engineering solution

Total accumulated dose (maximum values):

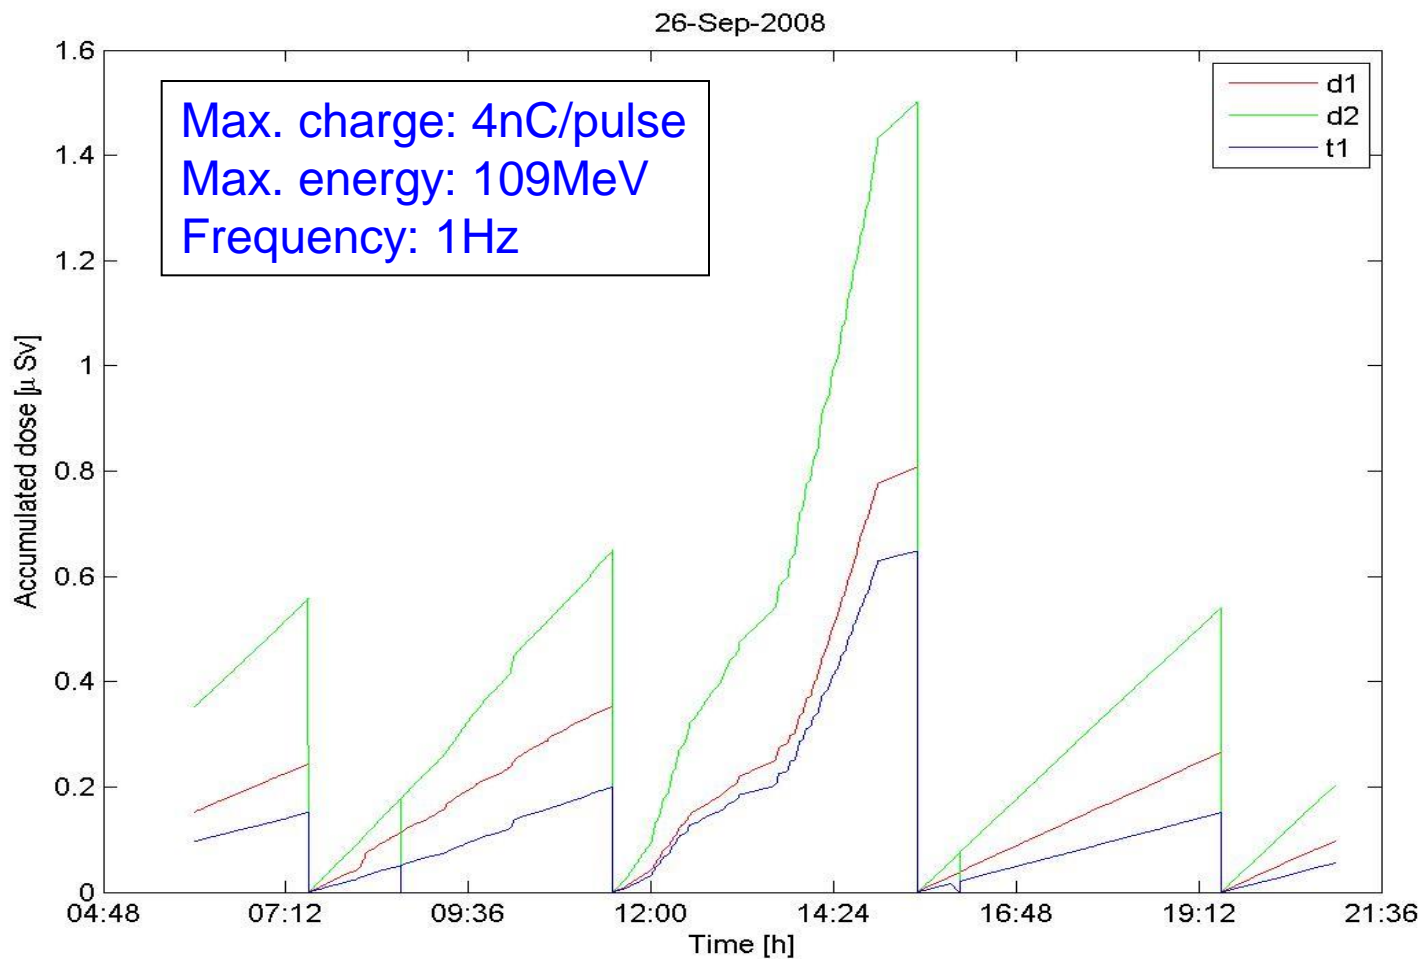

1. Engineering solution

❖ Integrated dose measured at the shield wall next to: BL16 & BL18 & BL20

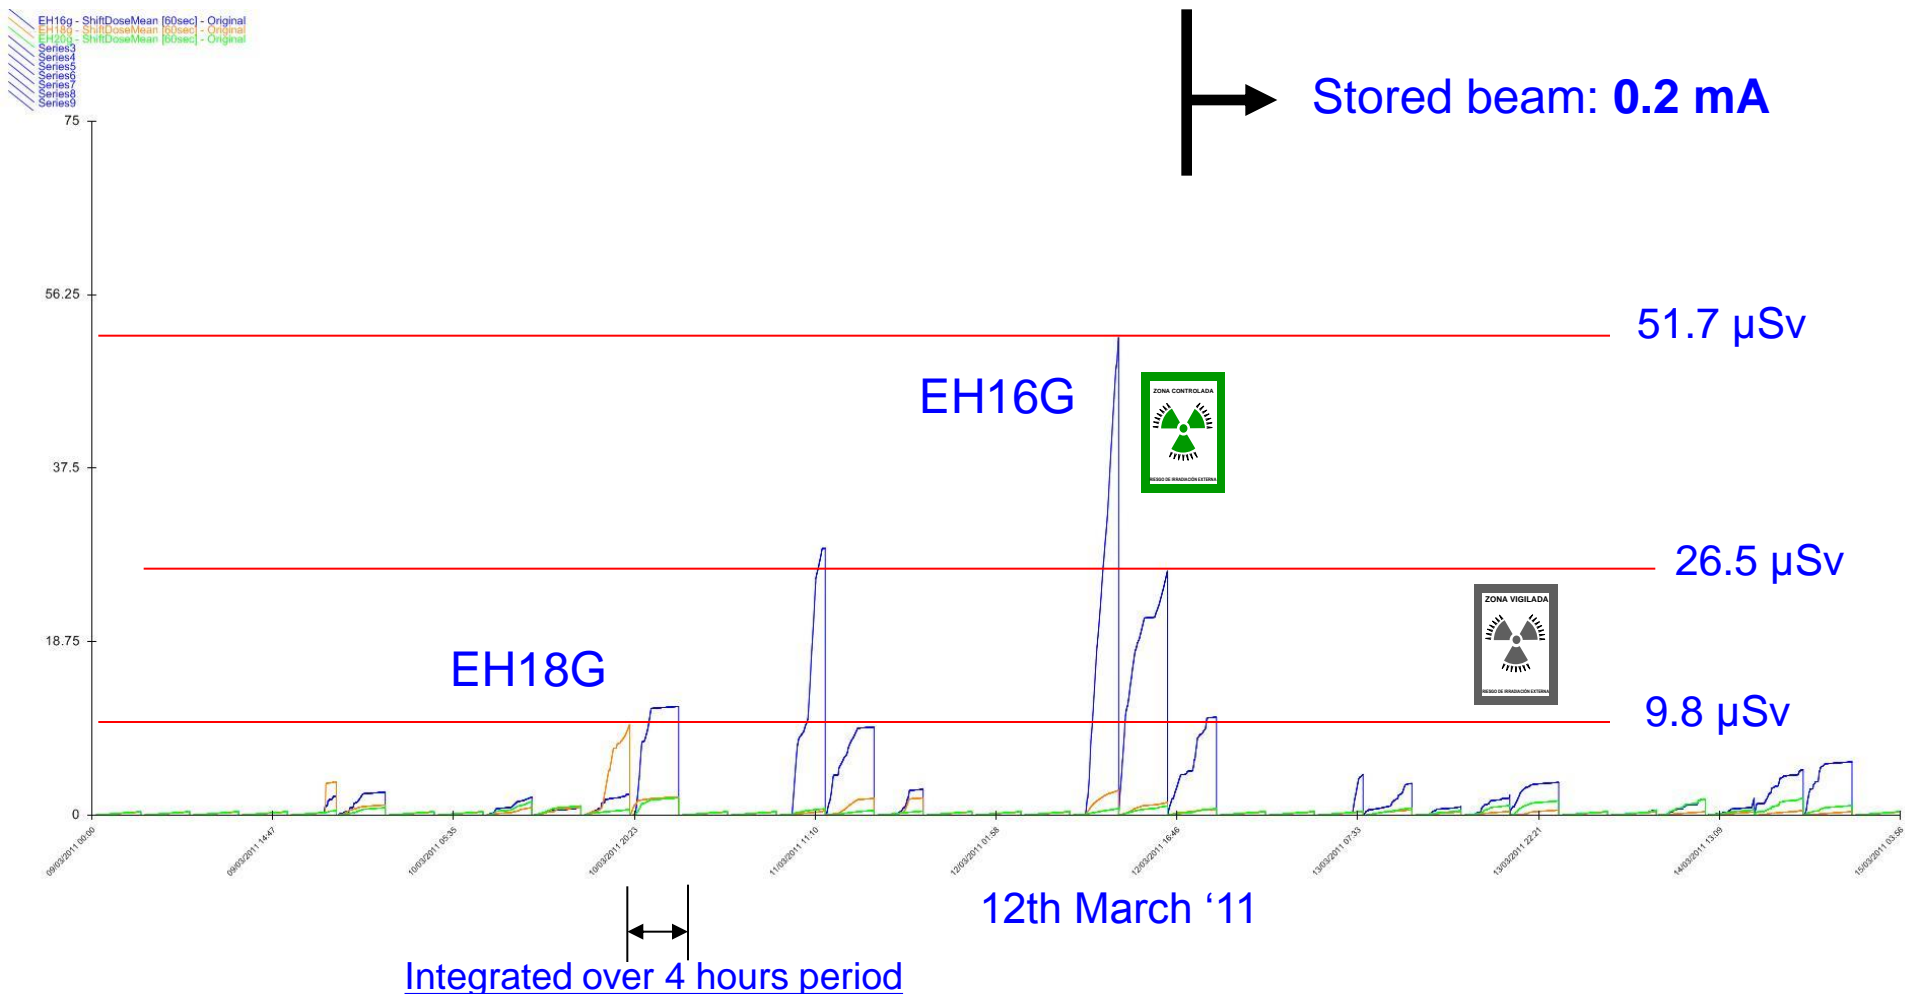


1. Engineering solution

❖ RADMON next to (integrated dose):

BL16 & TR03 (next to BL16) & BL27 & TR01 (next to BL27)

Stored beam: **100 mA**

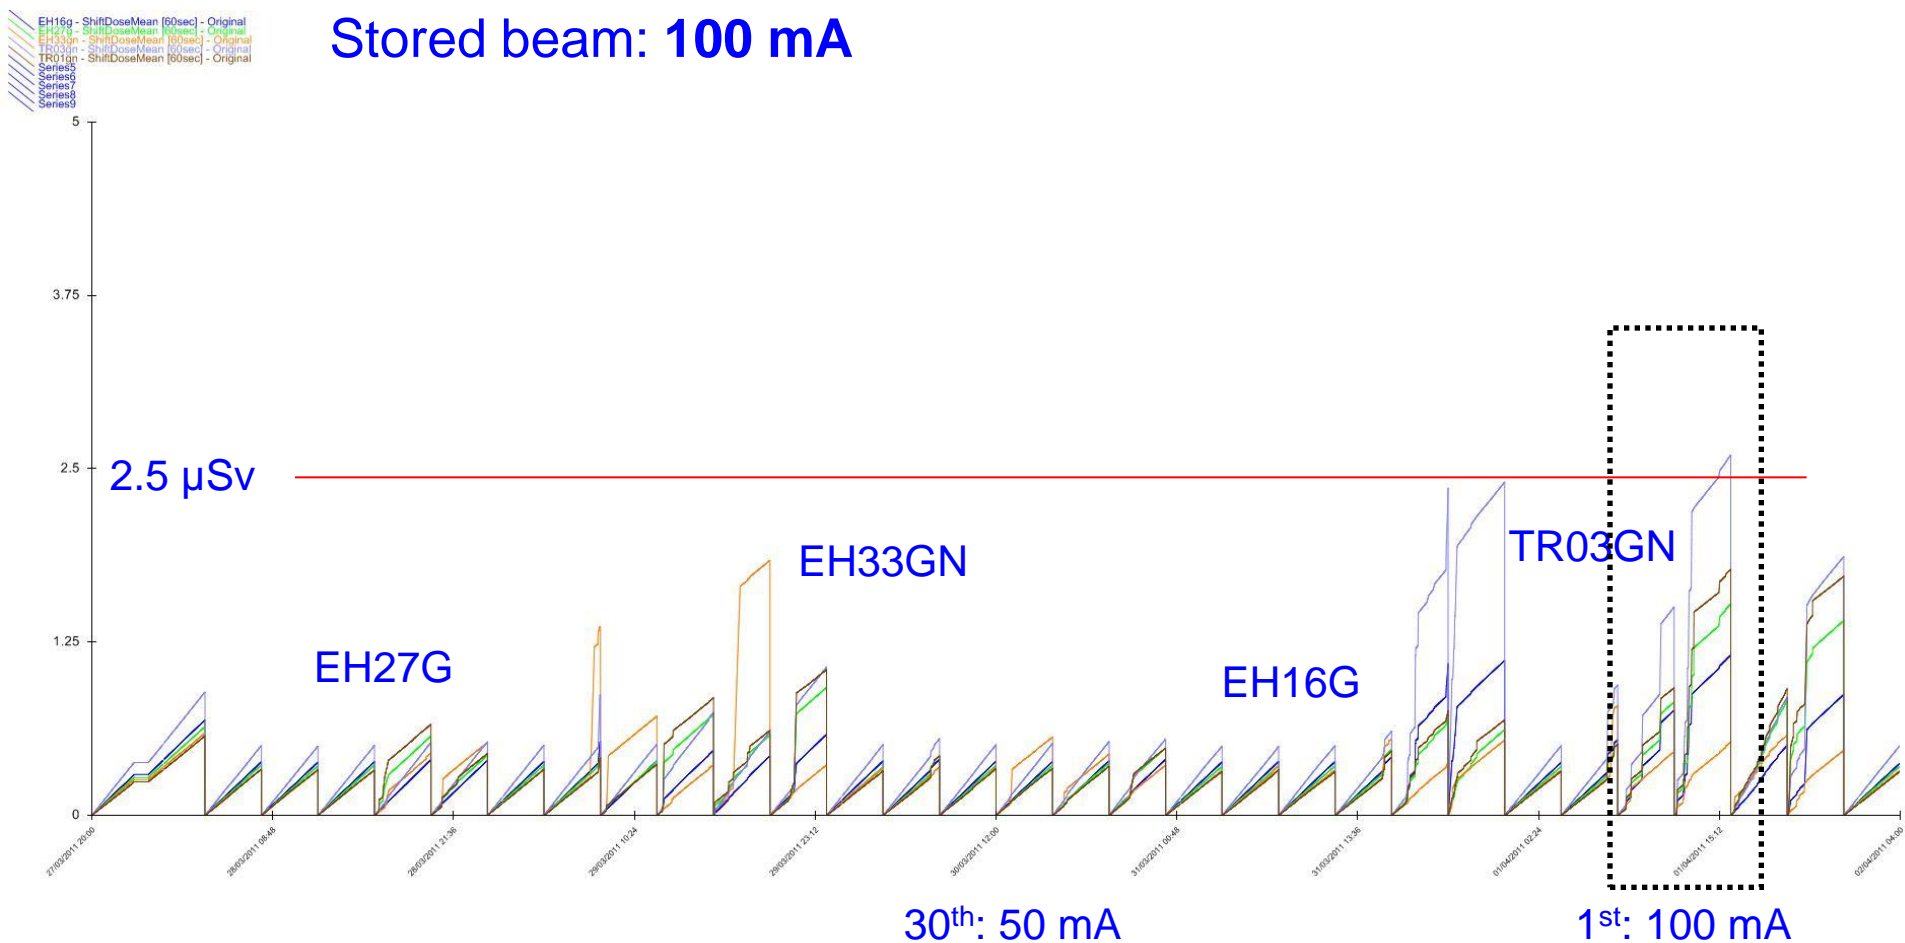


1. Engineering solution

❖ RADMON next to (gamma dose rate):

BL16 & TR03 (next to BL16) & BL27 TR01 (next to BL27)

EH16g - GammaDoseRate [2sec] - Original
EH27g - GammaDoseRate [2sec] - Original
EH33gn - GammaDoseRate [2sec] - Original
TR03gn - GammaDoseRate [2sec] - Original
TR01gn - GammaDoseRate [2sec] - Original
Series5
Series7
Series9
Series9

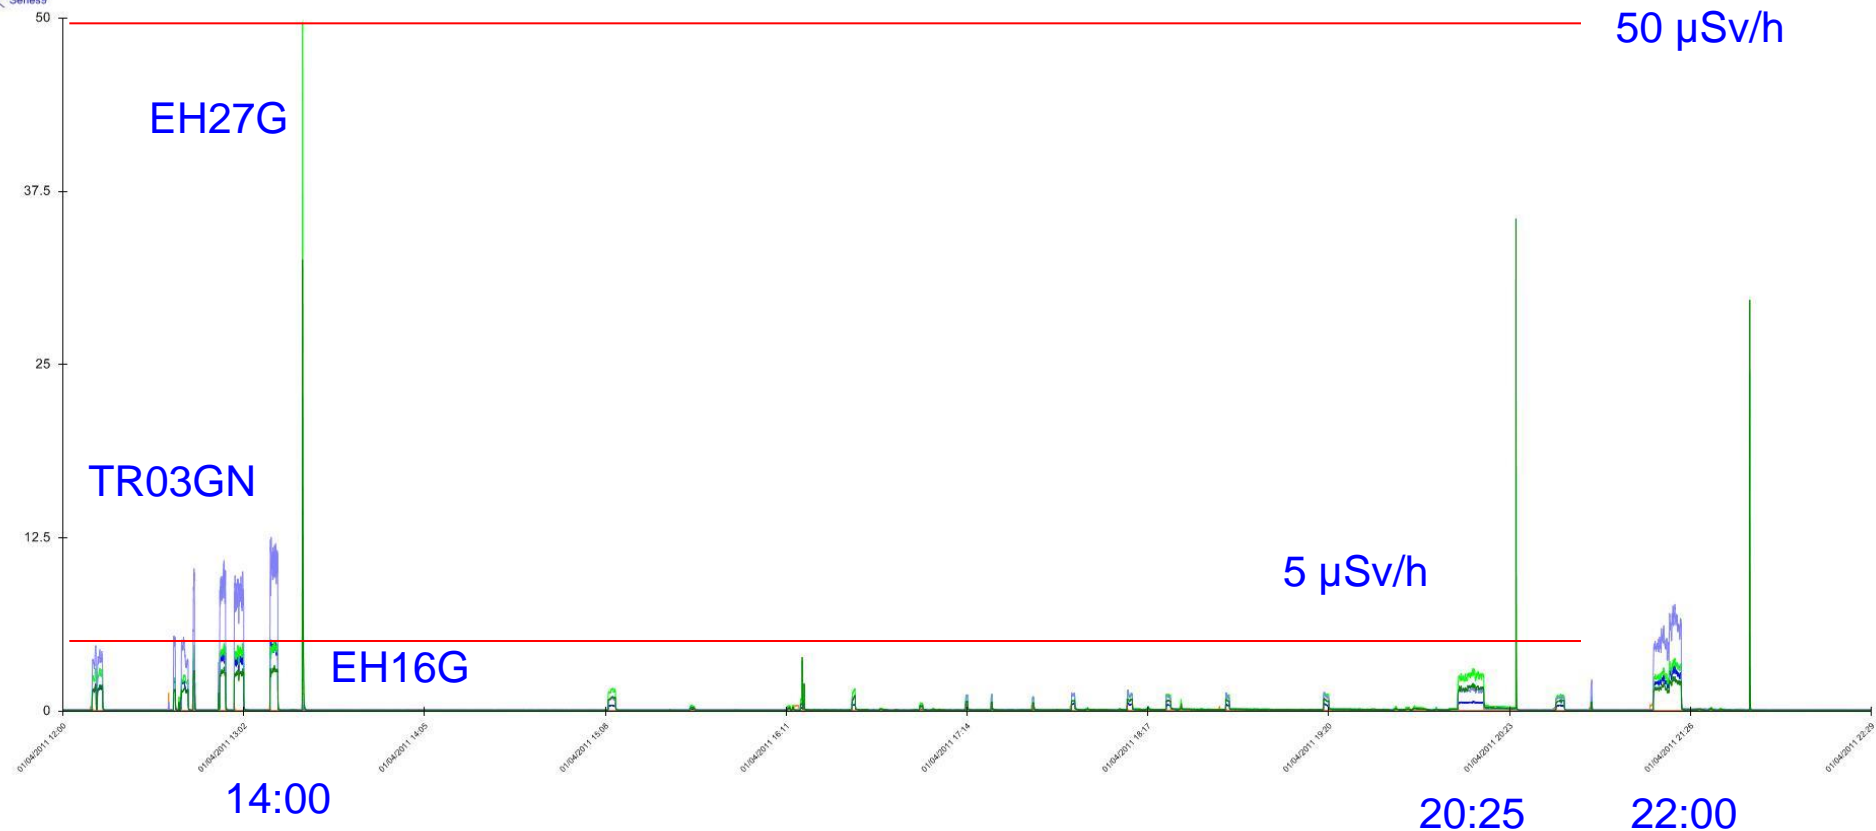

Radiation Safety – JUAS 2007, P. Berkvens

NCRP Report No 51: Radiation Protection Design Guidelines for 0.1-100 MeV Particle Accelerator Facilities. NCRP, 1979 - Although dated, still very useful. Scope limited to mostly radiation source terms and shielding. Concise, only technical information.

NCRP Report No 144: Radiation Protection for Particle Accelerator Facilities. NCRP, 2003.

It is a substantial revision and expansion of NCRP Report No. 51, the Report revises and expands on the earlier report and includes new information on source intensities, shielding, dosimetry, and the environmental aspects of particle accelerator operation. It is primarily concerned with radiological safety aspects that are special to the operation of particle accelerators having energies above about 5 MeV up to the highest energies available, while not neglecting low-energy neutron generators.

IAEA Report No. 188: Radiological Safety Aspects of the Operation of Electron Accelerators, IAEA, Vienna, 1979. - Scope limited to electron machines. Very detailed and comprehensive: all facets covered, except safety systems. Strongest points: source terms, shielding, yields (activation, ozone, noxious gases). Although dated, still a “must” for electron machines.

IAEA Report No. 283: Radiological Safety Aspects of the Operation of Proton Accelerators, IAEA, Vienna, 1988. - Equivalent to No. 188 for proton machines. More detailed, good reading on general issues, with some high-energy bias.

SLAC Report 327: Health Physics Manual of Good Practices for Accelerator Facilities. Stanford Linear Accelerator Center, - Written by a committee from DOE accelerator labs - bias towards large, high-energy facilities. Little technical detail, but strong on operational issues, including safety systems. Certain aspects not found elsewhere; useful general reading.

Landolt-Borstein Compendium: Shielding Against High Energy Radiation, 1990, Springer- Verlag - Written by former members of the CERN Radiation Protection group (Fasso et al). Very expensive, availability limited. Encyclopedic approach - compilation of large amounts of available data. Not good for general reading and learning, but a valuable reference for specialists.

A. H. Sullivan: A Guide to Radiation and Radioactivity Levels near High Energy Particle Accelerators, 1992, Nucl. Technology Publishing - Small “cookbook” with limited scope, but very practical. Essence distilled to rules-of-thumb and simple formulae.

ICRP Publication No 60: 1990 Recommendations of the International Commission on Radiological Protection, Oxford, 1991, Pergamon Press – Contains the latest recommendations on quantities and units for radiation protections, in particular the concepts of equivalent dose and effective dose.

ICRP Publication No 103: 2007 The 2007 Recommendations of the International Commission on Radiological Protection – It is an update of the No 60 and also include an approach for developing a framework to demonstrate radiological protection of the environment.

✓ *Many Thanks for your attention!*