
Medical Applications of Modern Physics

Marco Silari
CERN, Geneva, Switzerland
marco.silari@cern.ch

Medical Physics

=

A branch of applied physics concerning
the application of physics to medicine

or, in other words

The application of physics techniques to the
human health

Physics discoveries

Tools for physics applied to medicine

Medical imaging

X-ray CT

PET and PET/CT

Photon/electron radiation therapy

Hadron therapy

Physics discoveries

Tools for physics applied to medicine

Medical imaging


X-ray CT

PET and PET/CT

Photon/electron radiation therapy

Hadron therapy

The beginnings of modern physics and of medical physics

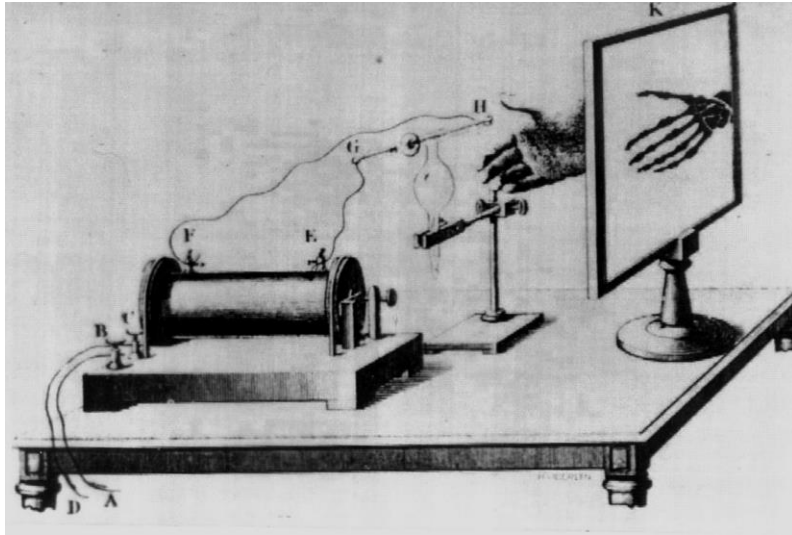

1895

Discovery of X rays

Wilhelm C. Röntgen

1897

First treatment of tissue with X rays


Leopold Freund



J.J. Thompson

1897

"Discovery" of the electron

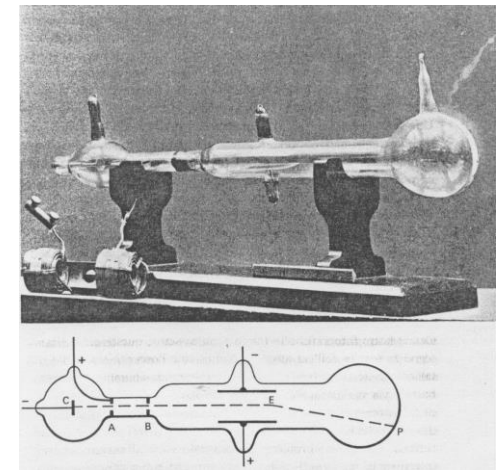

The beginnings of modern physics and of medical physics




**Henri Becquerel
(1852-1908)**

1896

Discovery of natural
radioactivity

Thesis of Mme. Curie – 1904


α , β , γ in magnetic field

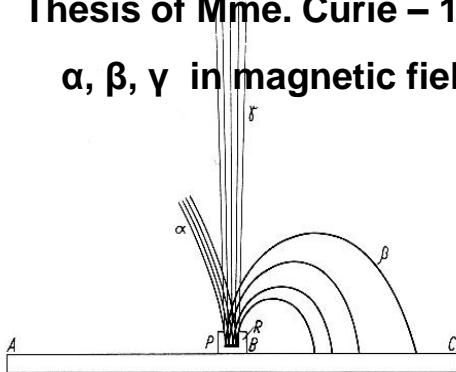

Hundred years ago

1898


Discovery of polonium
and radium

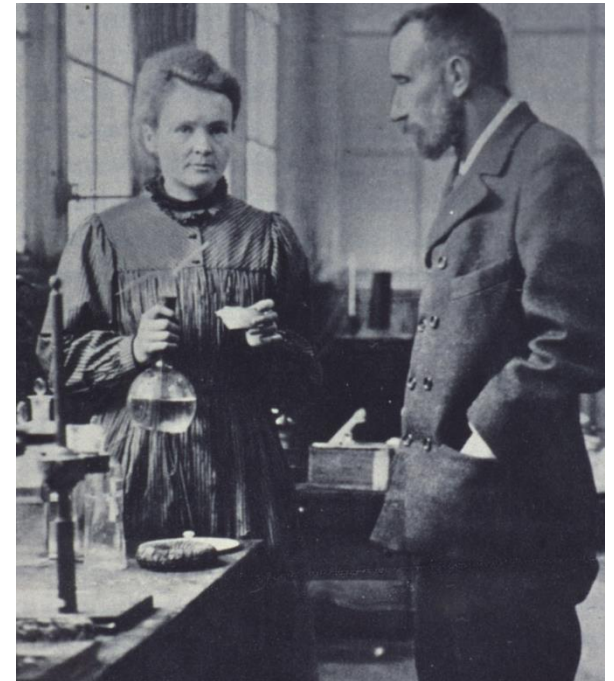

**Marie Curie Pierre Curie
(1867 – 1934) (1859 – 1906)**

First practical application of a radioisotope

- **1911: first practical application of a radioisotope** (as *radiotracer*) by G. de Hevesy (a young Hungarian student working with naturally radioactive materials) in Manchester
- **1924:** de Hevesy, who had become a physician, used radioactive isotopes of lead as tracers in bone studies

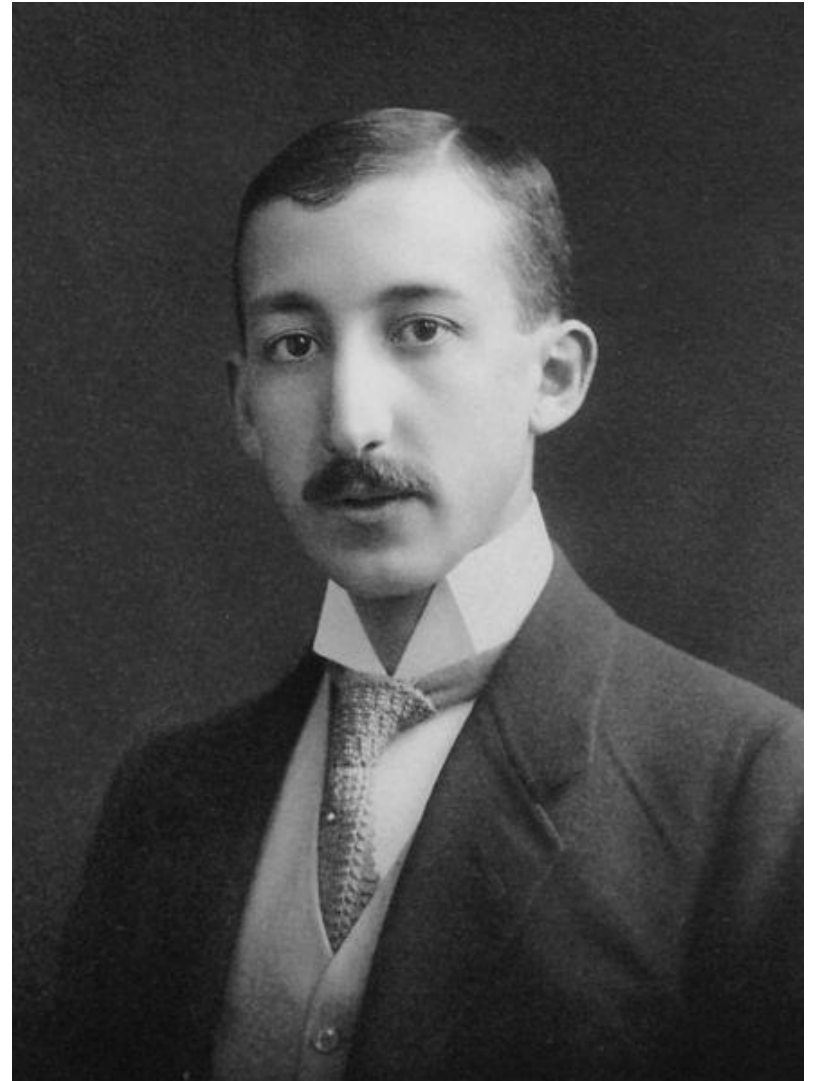


Tools for (medical) physics: the cyclotron



1930

Invention of the cyclotron

Ernest Lawrence

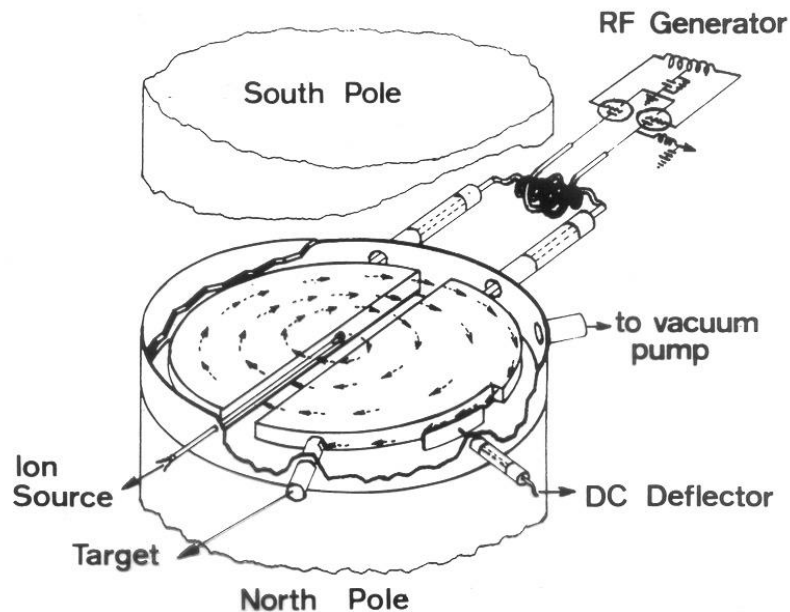


The beginnings of modern physics and of medical physics



James Chadwick
(1891 – 1974)

1932

Discovery of the neutron

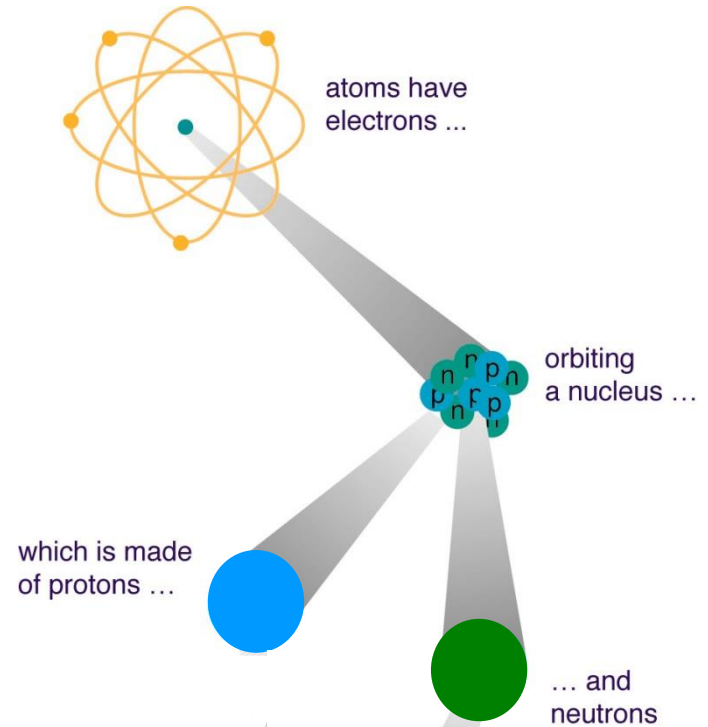


Cyclotron + neutrons = first attempt of radiation therapy with fast neutrons at LBL (R. Stone and J. Lawrence, 1938)

The beginnings of modern physics and of medical physics

1932


Discovery of the positron

C. D. Anderson

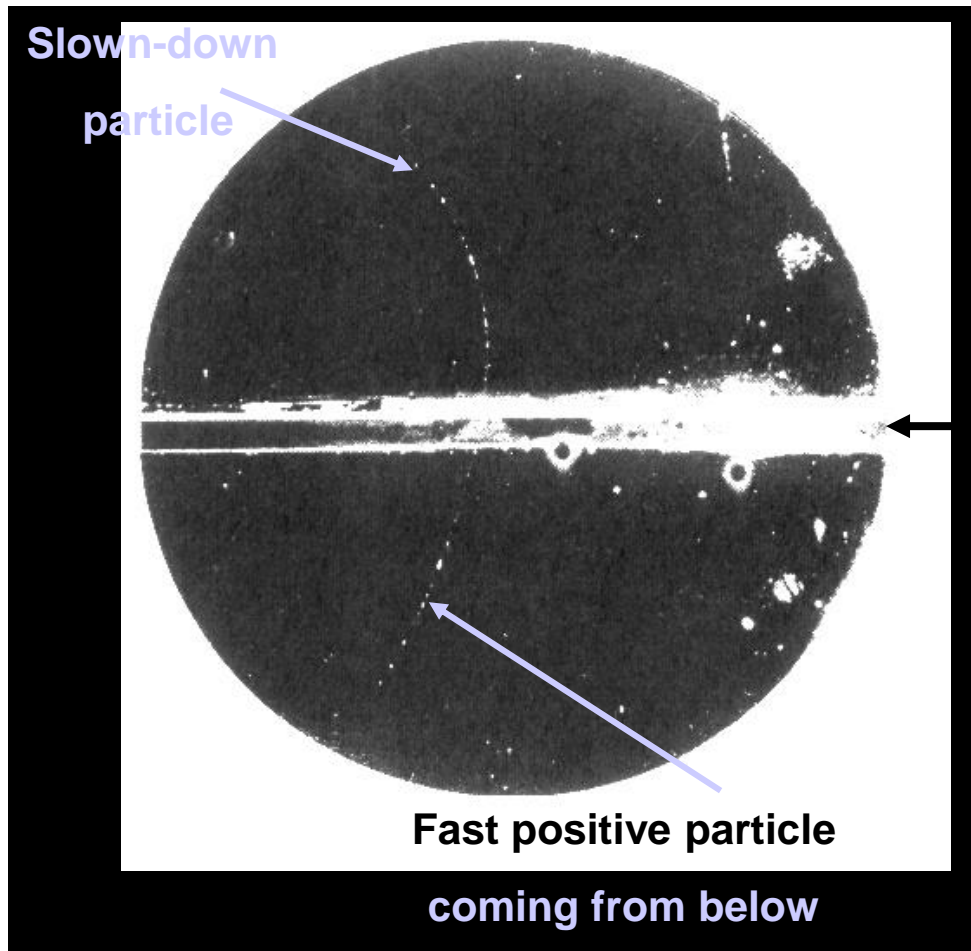

Layer of lead

Inserted in a cloud chamber

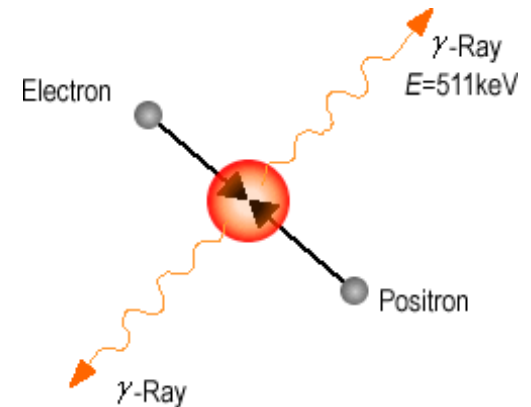


Historical development of radioisotopes for medicine

- **1932:** the invention of the cyclotron by E. Lawrence makes it possible to produce radioactive isotopes of a number of biologically important elements
- **1941:** first medical cyclotron installed at Washington University, St Louis, for the production of radioactive isotopes of phosphorus, iron, arsenic and sulphur
- **After WWII:** following the development of the fission process, most radioisotopes of medical interest begin to be produced in nuclear reactors
- **1951:** Cassen et al. develop the concept of the rectilinear scanner
- **1957:** the $^{99}\text{Mo}/^{99\text{m}}\text{Tc}$ generator system is developed by the Brookhaven National Laboratory
- **1958:** production of the first gamma camera by Anger, later modified to what is now known as the Anger scintillation camera, still in use today

Tools for (medical) physics: the electron linac

Sigmur Varian

William W. Hansen

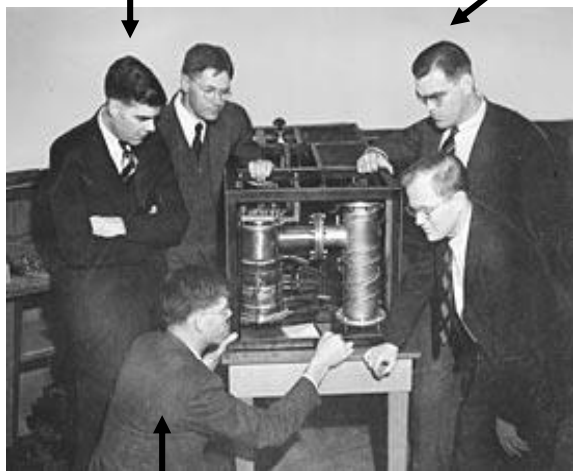


Russell Varian

1939

Invention of the klystron

1950's: development of compact linear electron accelerators by various companies

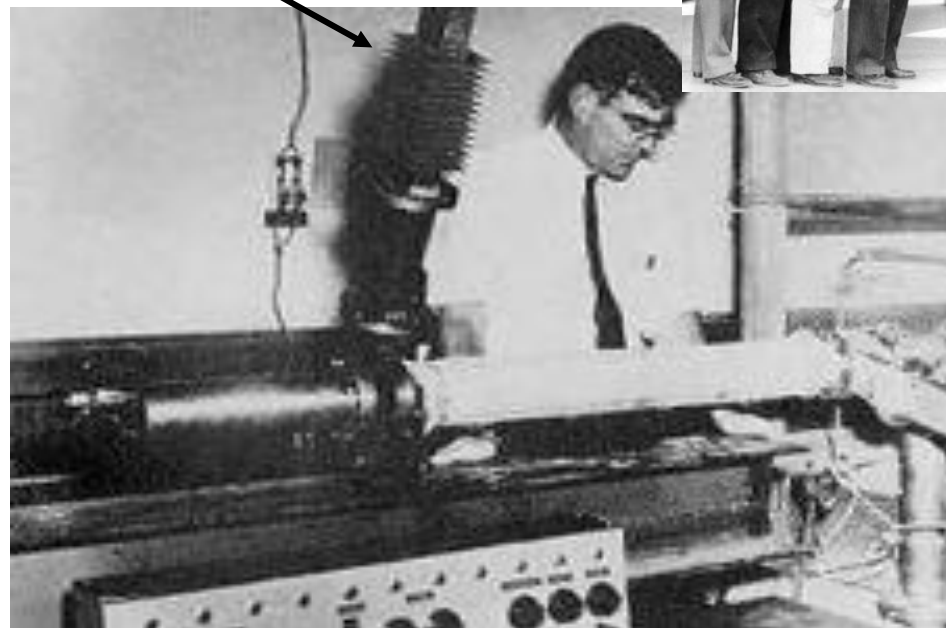


1947

first linac for electrons
4.5 MeV and 3 GHz

Tools for (medical) physics: the synchrotron


1945: E. McMillan and V.J.Veksler

discover the
principle of phase stability

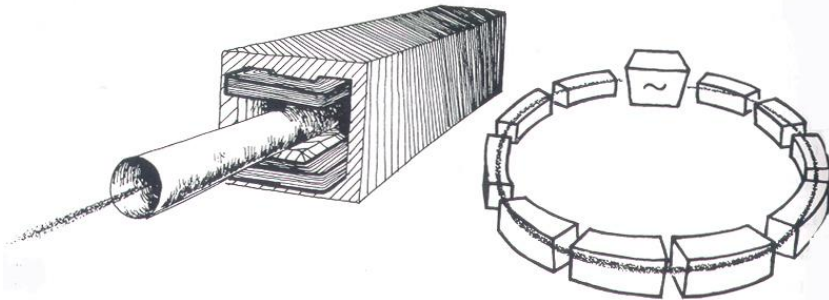

1 GeV electron synchrotron

Frascati - INFN - 1959

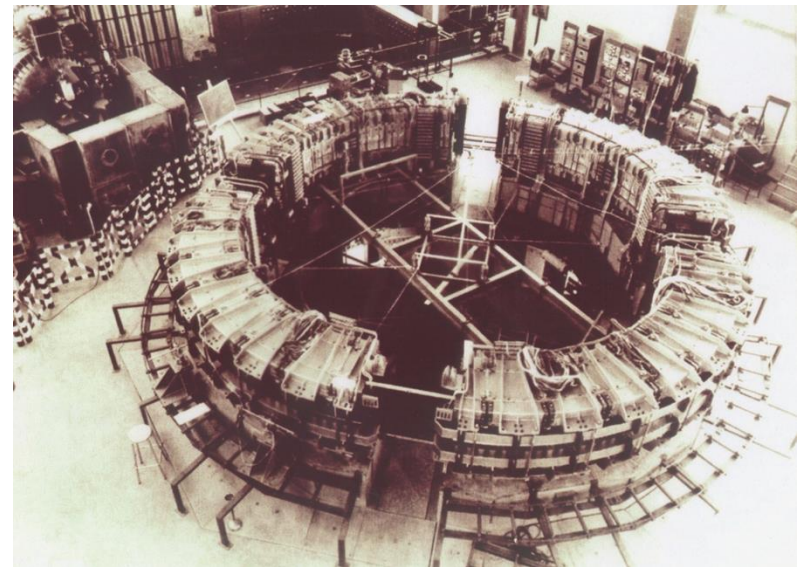


6 GeV proton synchrotron

Bevatron - Berkeley - 1954

CERN accelerators

Large Hadron Collider
7 TeV + 7 TeV
Start in 2008

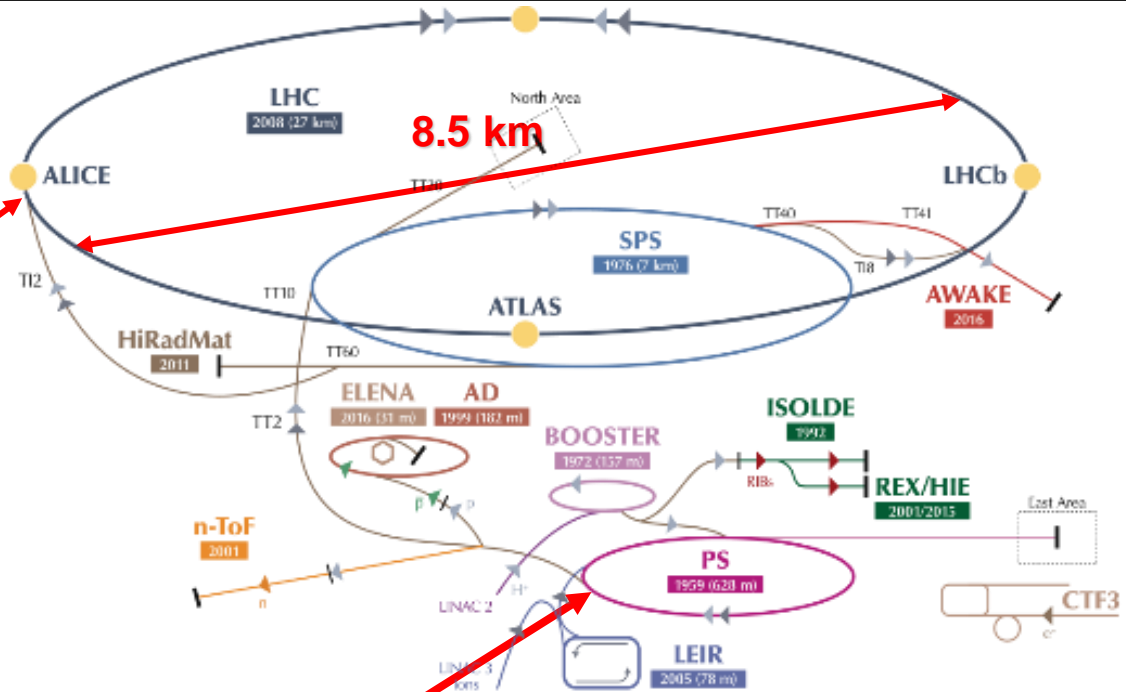

In 1952 the “strong-focusing” method
invented at BNL (USA)
was chosen for the CERN PS

Physics discoveries

Tools for physics applied to medicine

Medical imaging




X-ray CT

PET and PET/CT




Photon/electron radiation therapy

Hadron therapy

Medical imaging



TECHNIQUE		YEAR	ENERGY	PHYSICAL PROPERTY	IMAGING
RADIOLOGY	X RAYS IMAGING	1895	X RAYS	ABSORPTION	
ECHOGRAPHY	ULTRASOUND IMAGING	1950	US	REFLECTION TRANSMISSION	
NUCLEAR MEDICINE	RADIOISOTOPE IMAGING	1950	γ RAYS	RADIATION EMISSION	

Medical imaging

TECHNIQUE		YEAR	ENERGY	PHYSICAL PROPERTY	IMAGING	
X RAYS COMPUTERIZED TOMOGRAPHY	CT	1971	X RAYS	ABSORPTION		MORPHOLOGY
MAGNETIC RESONANCE IMAGING	MRI	1980	RADIO WAVES	MAGNETIC RESONANCE		MORPHOLOGY /FUNCTION
POSITRON EMISSION TOMOGRAPHY	PET	1973	γ RAYS	RADIATION EMISSION		FUNCTION


Emission versus transmission imaging

External versus internal radiation sources

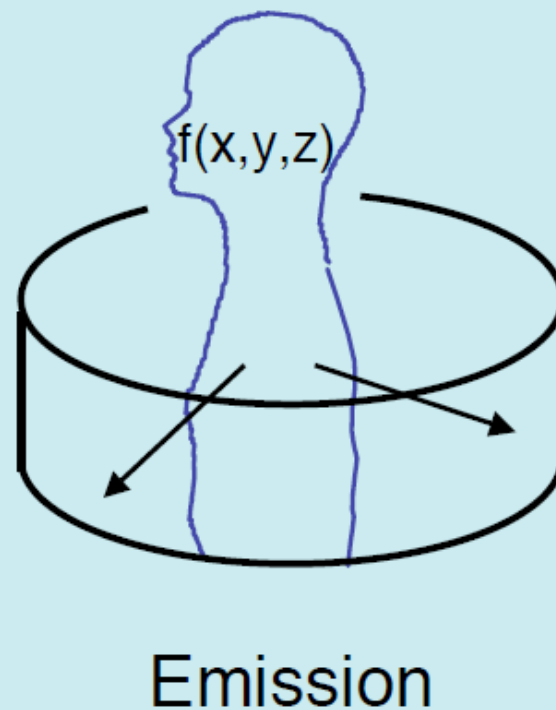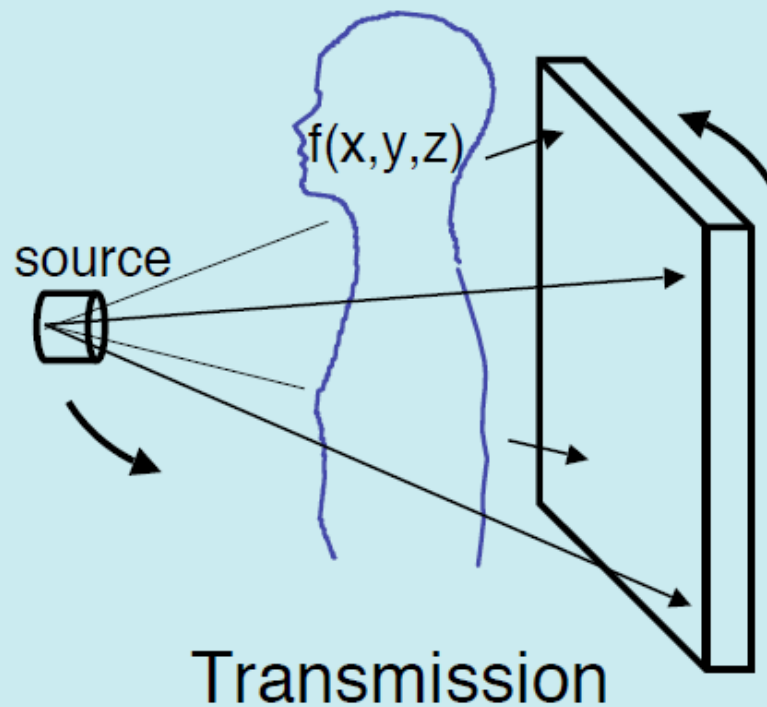

X-ray image versus CT scan

A conventional X-ray image is basically a **shadow**: you shine a “light” on one side of the body, and a piece of film on the other side registers the silhouette of the bones (to be more precise, **organs and tissues of different densities show up differently on the radiographic film**).

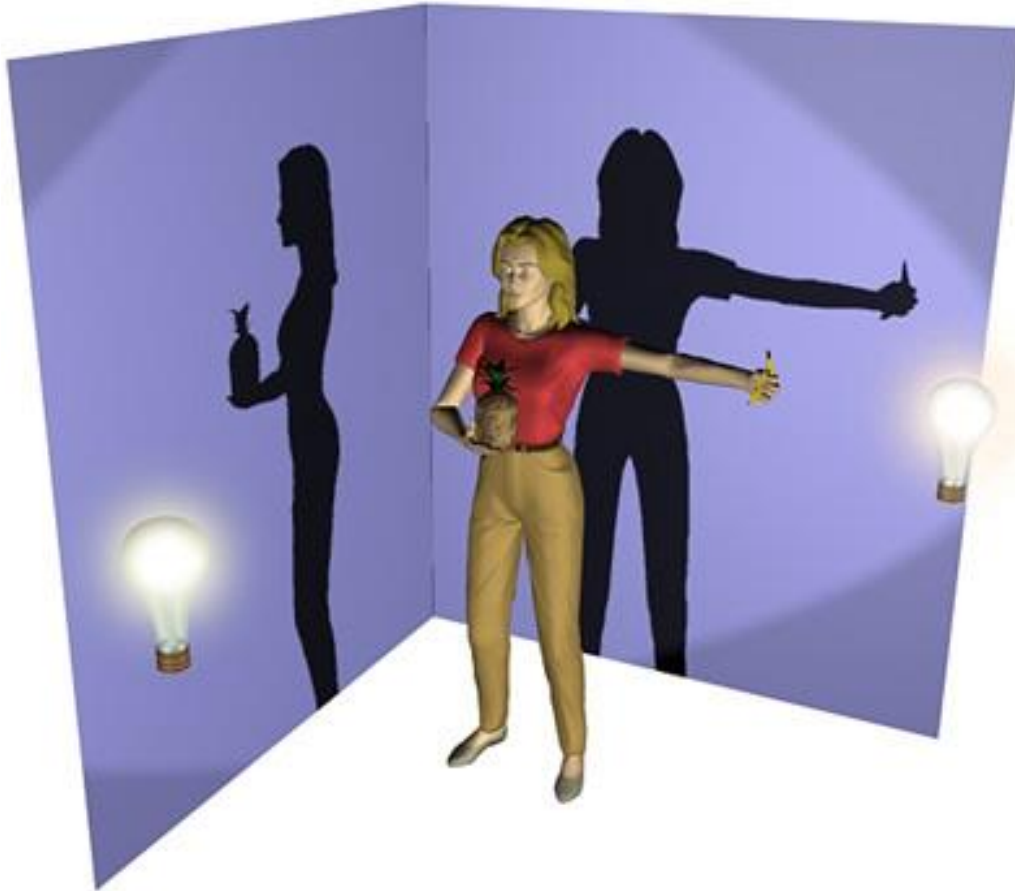


Shadows give an incomplete picture of an object's shape.

Look at the wall, not at the person. If there's a lamp in front of the person, you see the silhouette holding the banana, but not the pineapple as the shadow of the torso blocks the pineapple. If the lamp is to the left, you see the outline of the pineapple, but not the banana.



© 2002 HowStuffWorks

Computed tomography


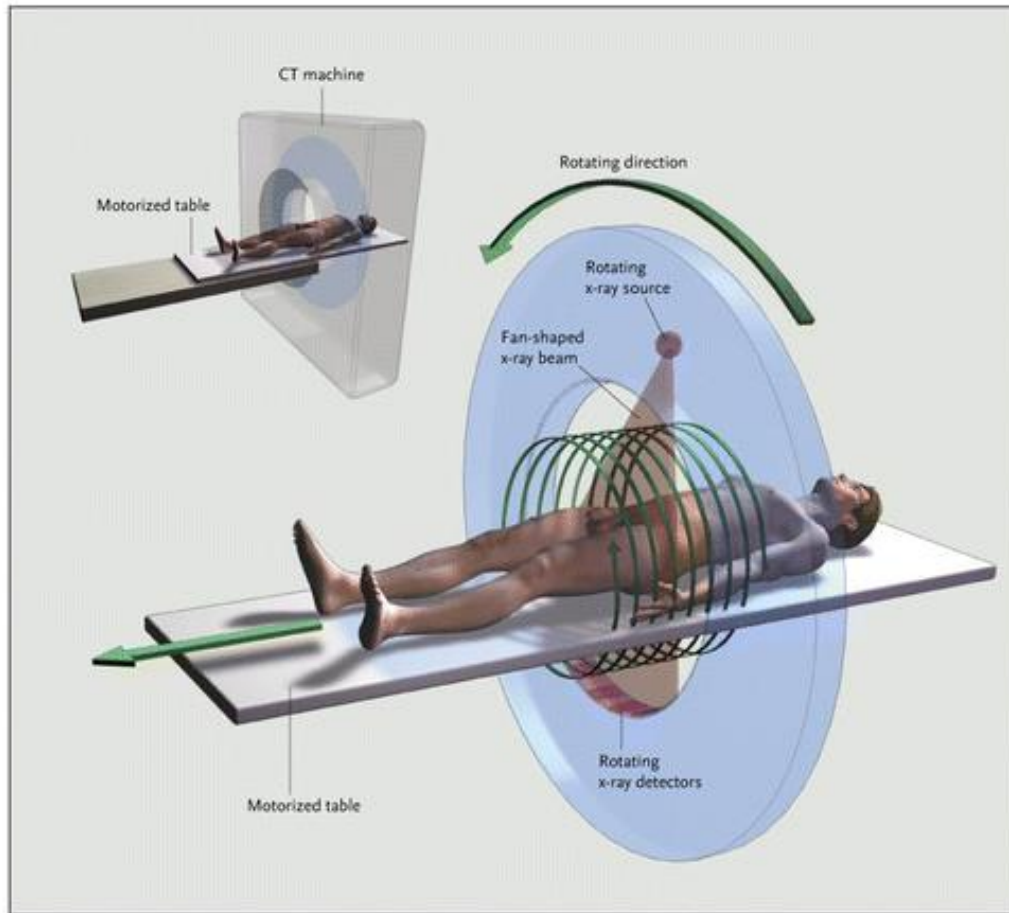


- The X-rays source rotates around the longitudinal axis of the body: it moves 360° around the patient, scanning from hundreds of different angles
- Opposite to the x-ray source, a series of detectors measure the radiation emerging from the body
- Each rotation scans a different body slice
- The couch moves to scan the next slice
- A computer analyses the data and reconstructs the **3D image** through mathematical algorithms.

Volumetric CT

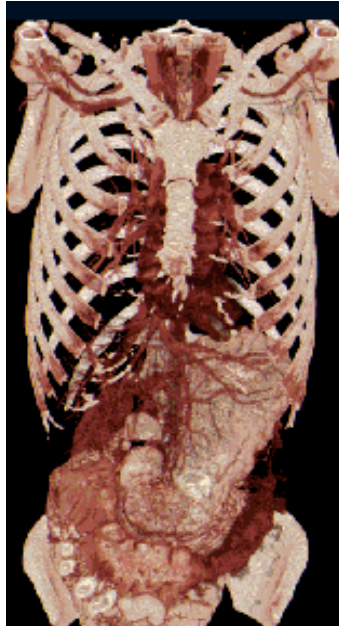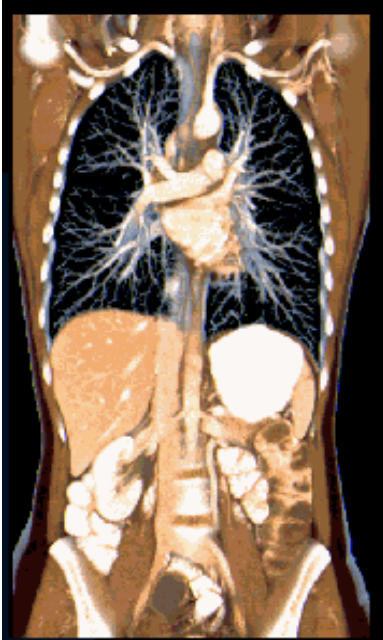


< 0.4 sec/rotation
Organ in a sec (17 cm/sec)
Whole body < 10 sec

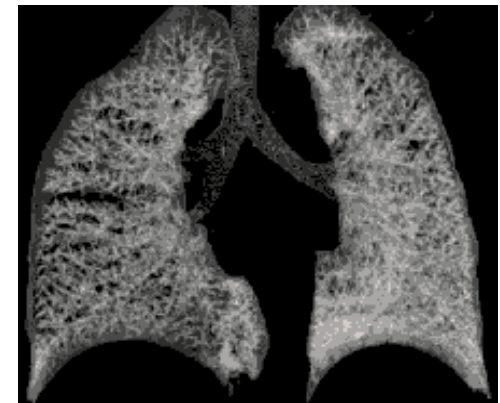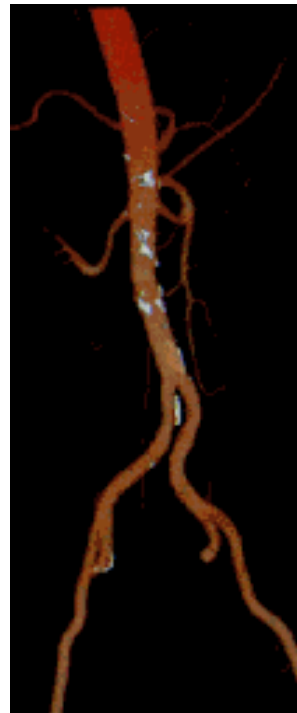




Cardiac CT






DYNAMIC CT ACQUISITION




ECG



PHASES OF A CARDIAC CYCLE

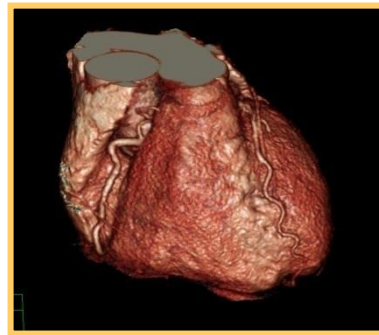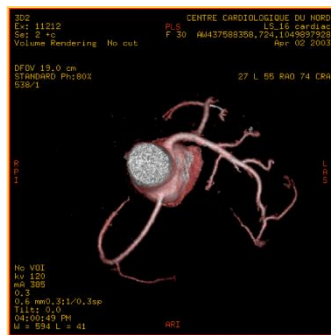

- EJECTION FRACTION
- CARDIAC OUTPUT
- REGIONAL WALL MOTION
- ..



FUNCTIONAL PARAMETERS


VOLUME RENDERED IMAGE OF HEART AND VESSELS

All **radionuclides** commonly administered to patients in nuclear medicine are *artificially* produced

Three production routes:

- **(n, γ) reactions (nuclear reactor)**: the resulting nuclide has the same chemical properties as those of the target nuclide
- **Fission (nuclear reactor)** followed by separation
- **Charged particle induced reaction (cyclotron)**: the resulting nucleus is usually that of a different element

Positron Emission Tomography (PET)

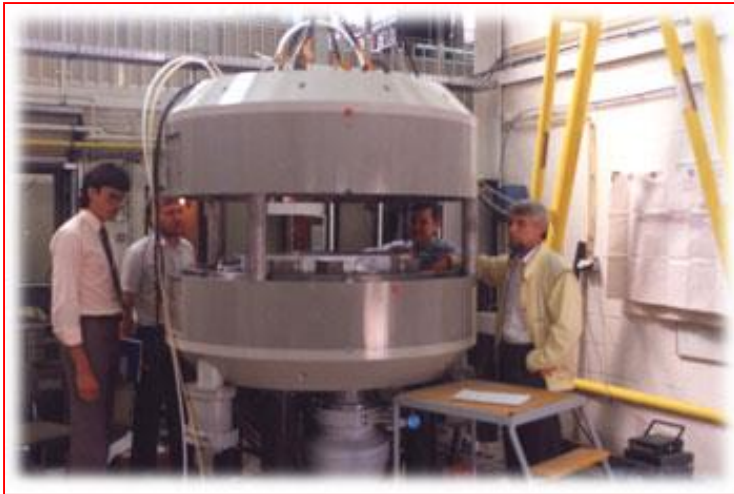


Cyclotron

Radiochemistry





ISOTOPES	Half-Life	
11-C	20.4 min,	"natural"
13-N	10.0 min	"natural"
15-O	2.0 min	"natural"
18-F	109.8 min	"pseudo-natural"

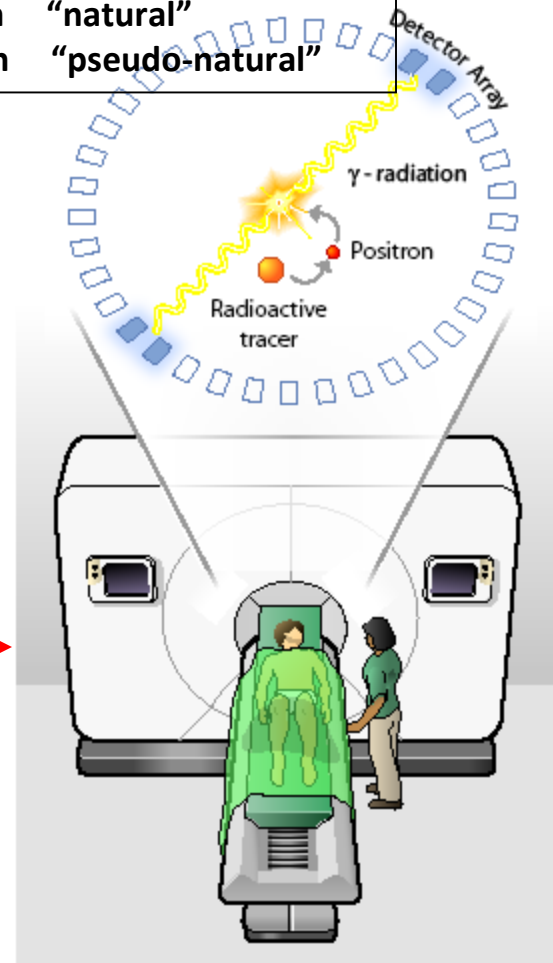

PET camera

Positron Emission Tomography (PET)

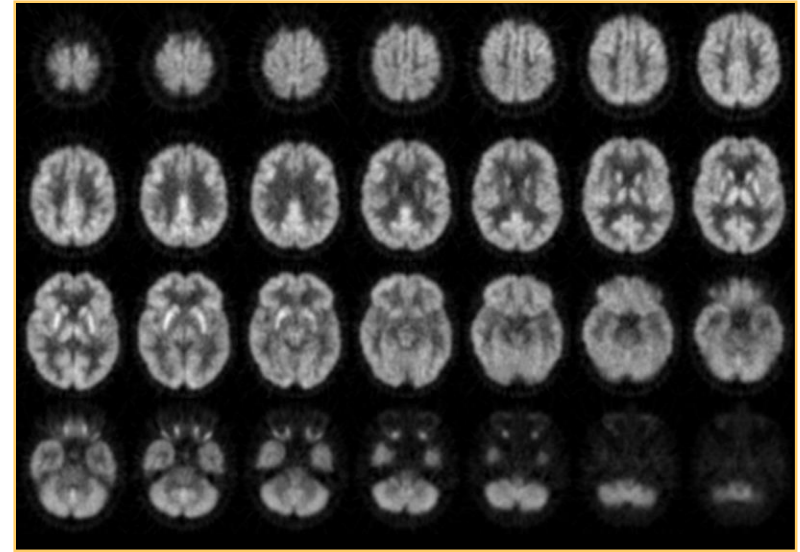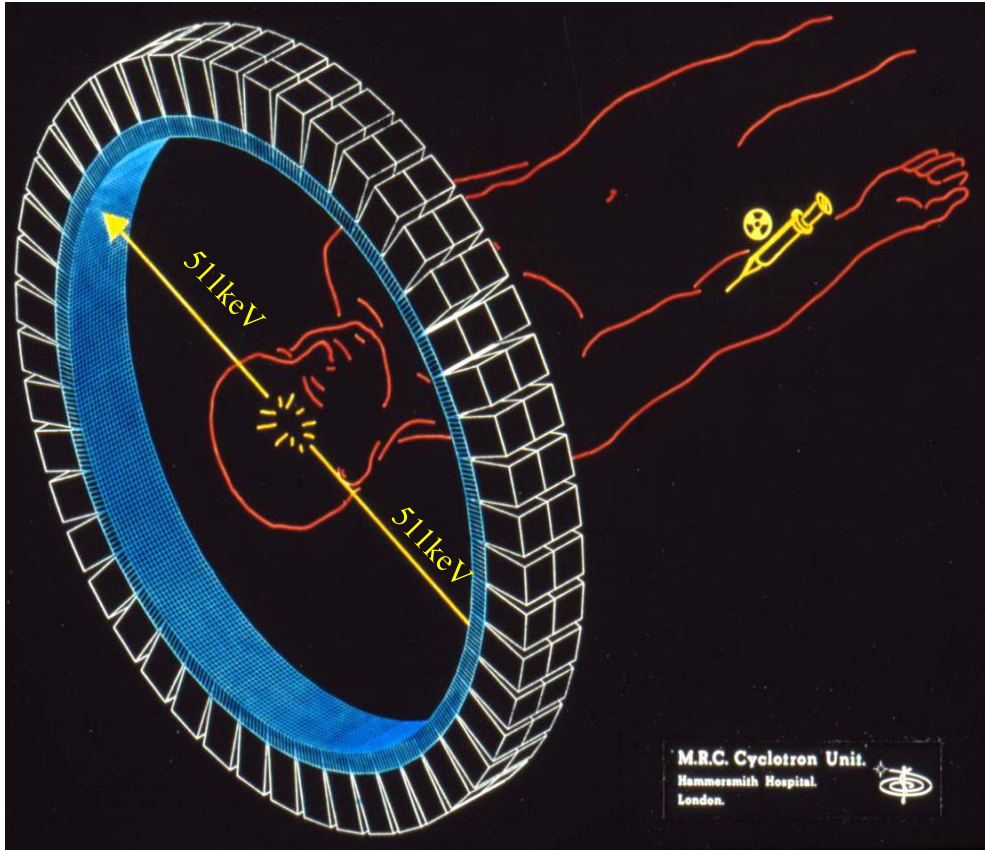

COVERAGE:

~ 15-20 cm

SPATIAL RESOLUTION:

~ 5 mm



SCAN TIME to cover an entire organ:

~ 5 min

CONTRAST RESOLUTION:

depends on the radiotracer

PET functional receptor imaging

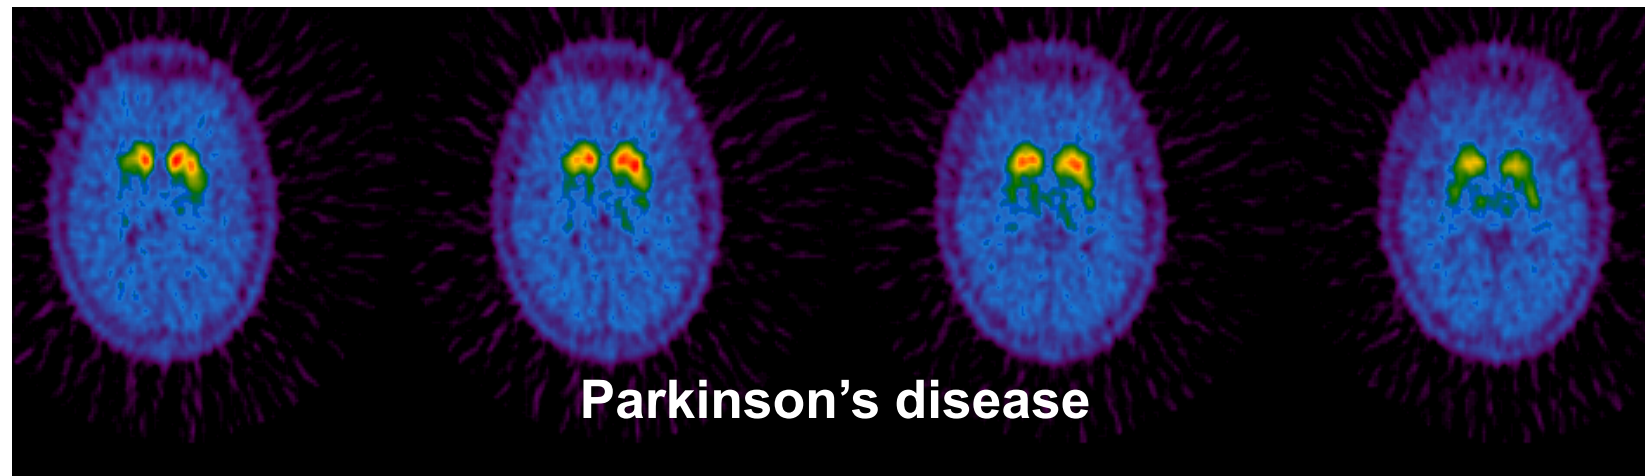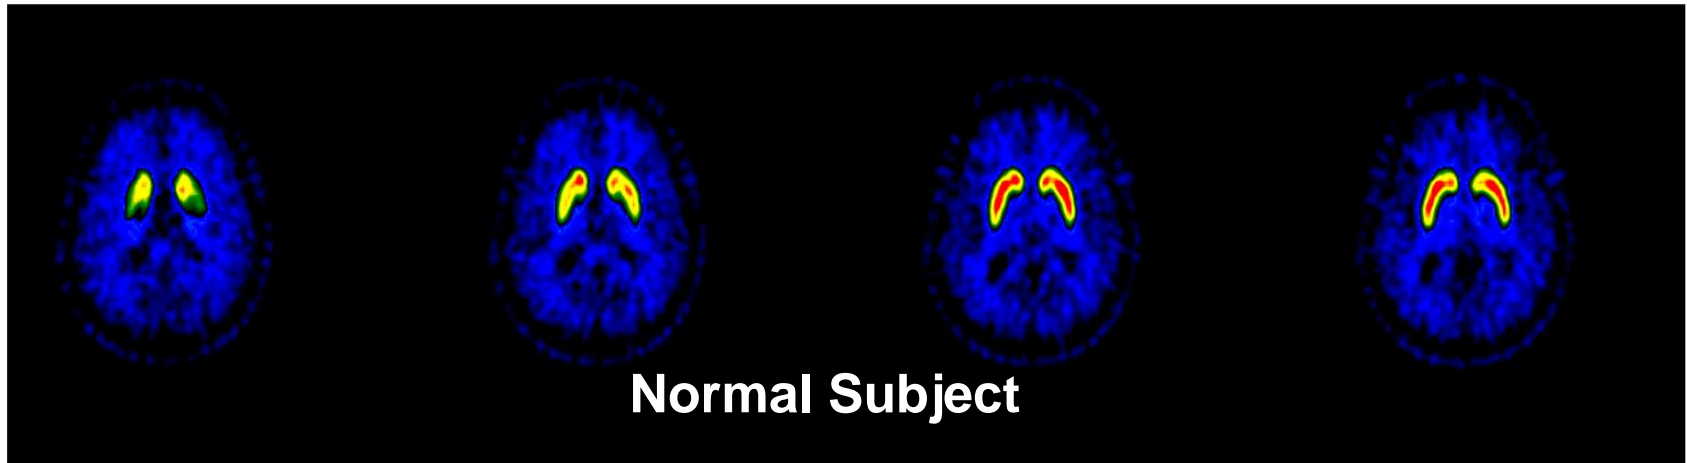


$[^{11}\text{C}]$ FE-CIT

Courtesy HSR MILANO


PET coverage and axial sampling

FIRST GENERATION PET

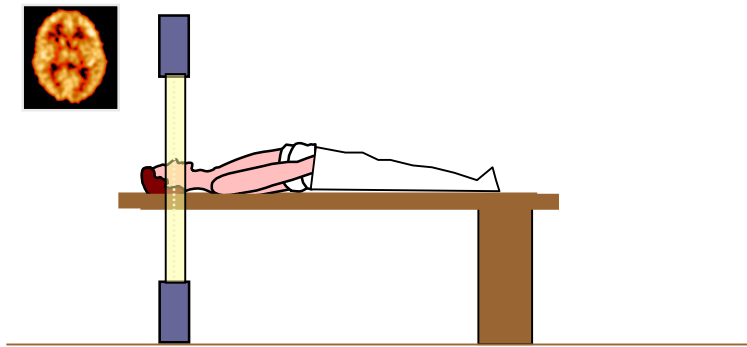

1 SLICE – 2 cm



CURRENT GENERATION PET

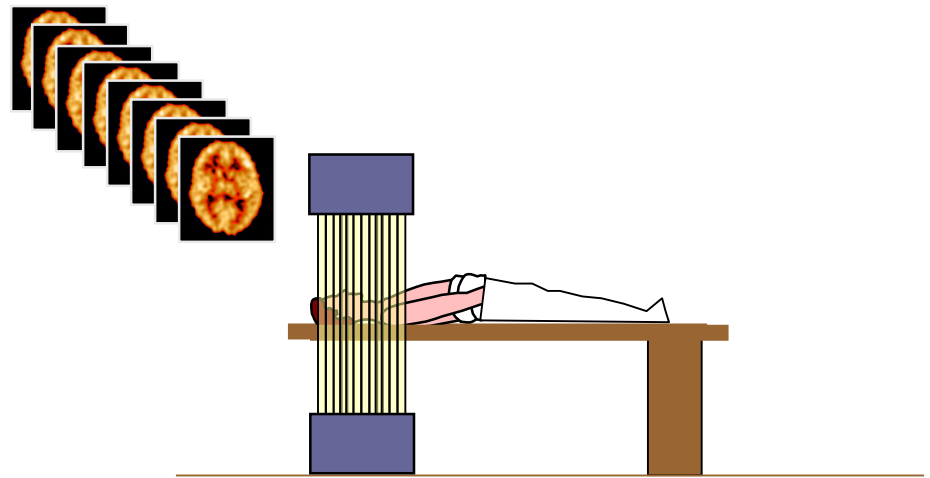

> 40 SLICES – 6 mm
Axial FOV: 15 – 20 cm

PET: total body studies


TRANSAXIAL
IMAGES

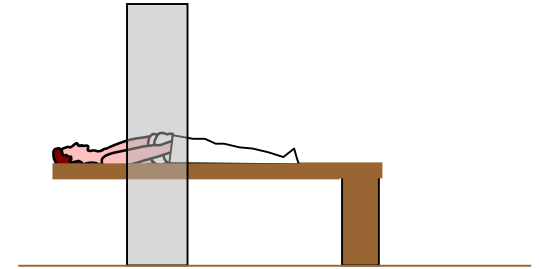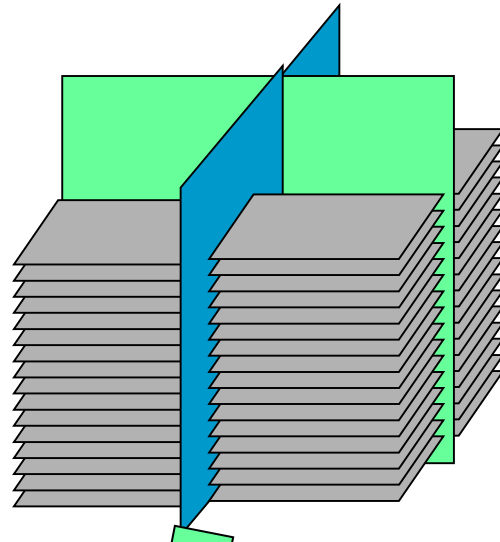


CORONAL




SAGITTAL

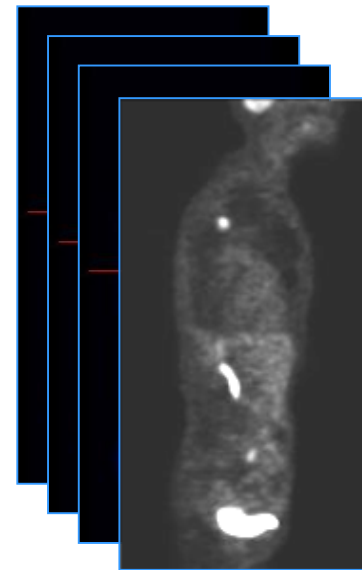


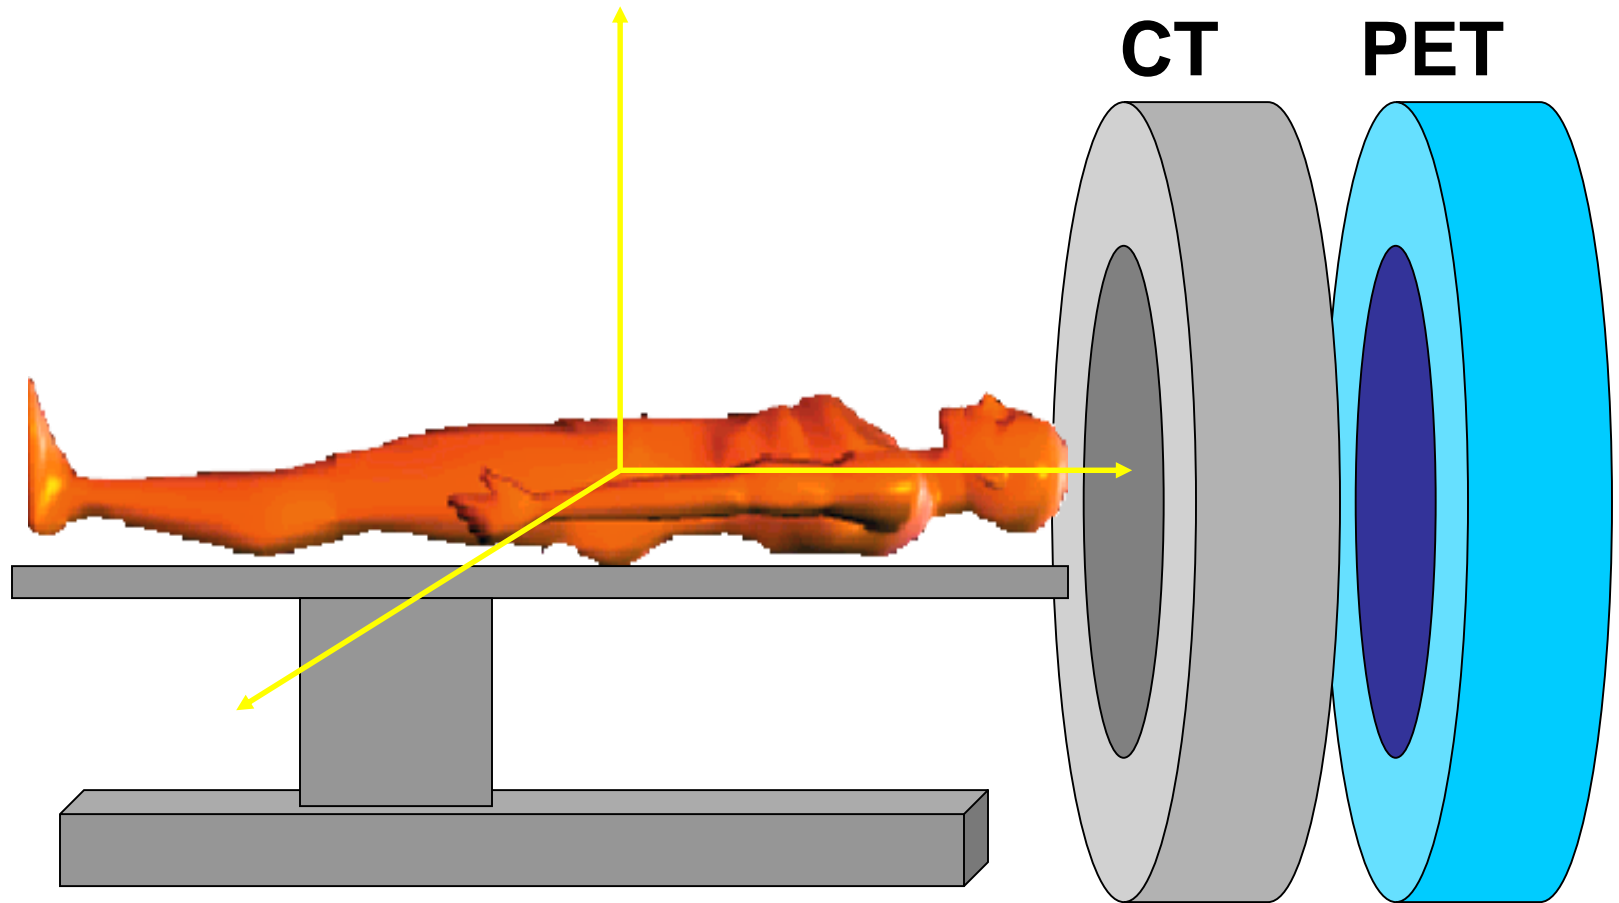


PET/CT scanner

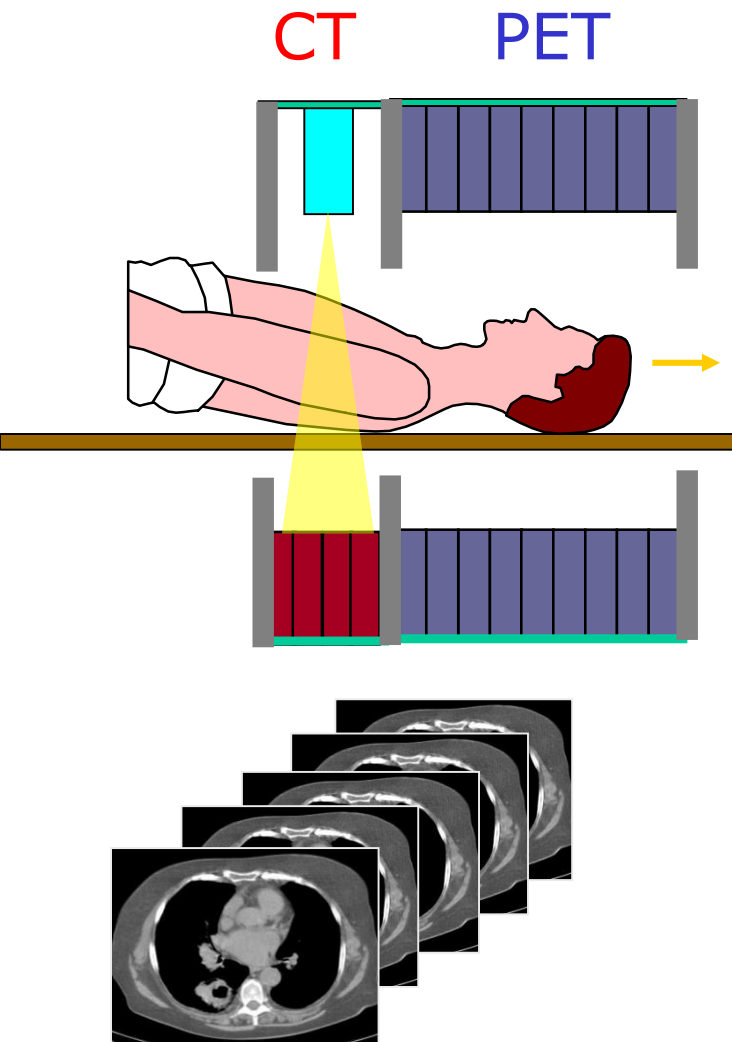


Courtesy HSR MILANO

PET/CT scanner

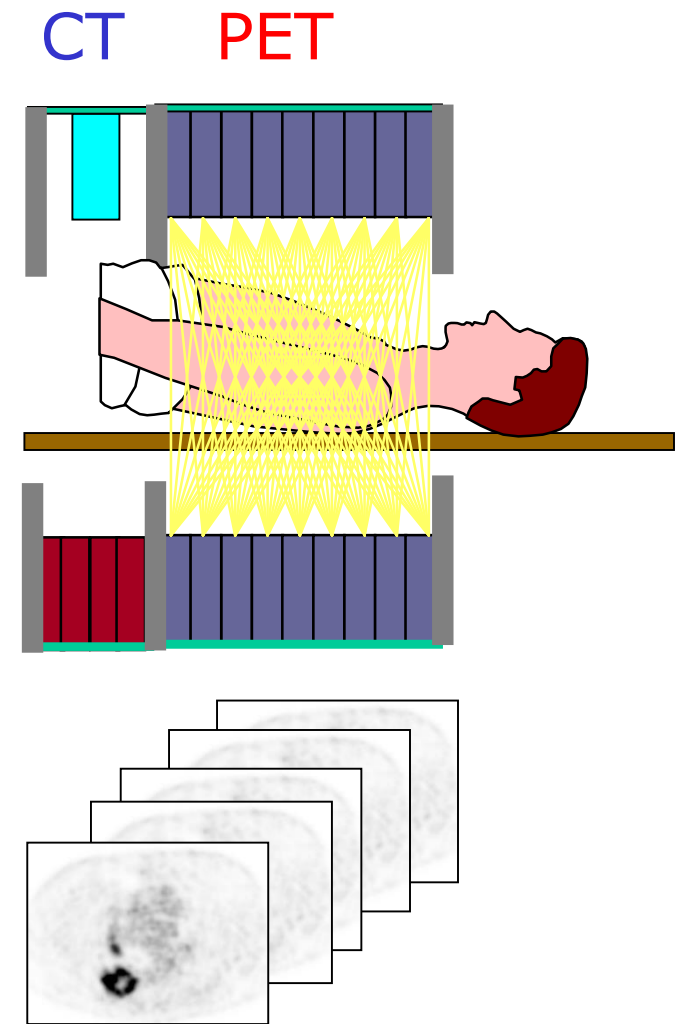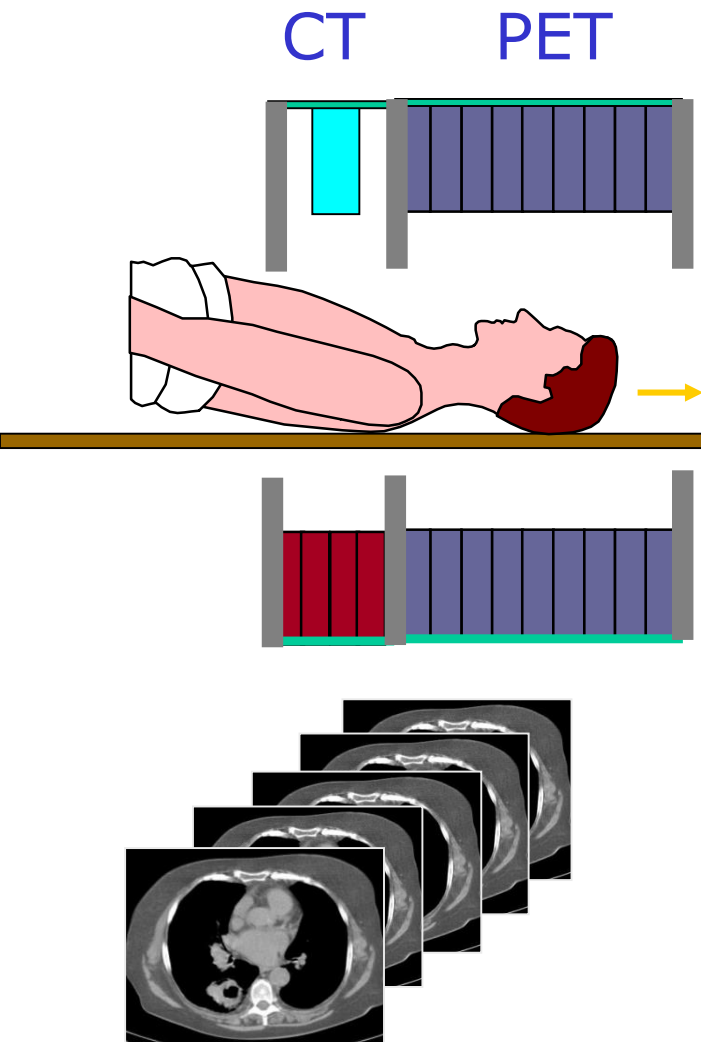


Courtesy HSR MILANO

^{18}F -FDG PET/CT

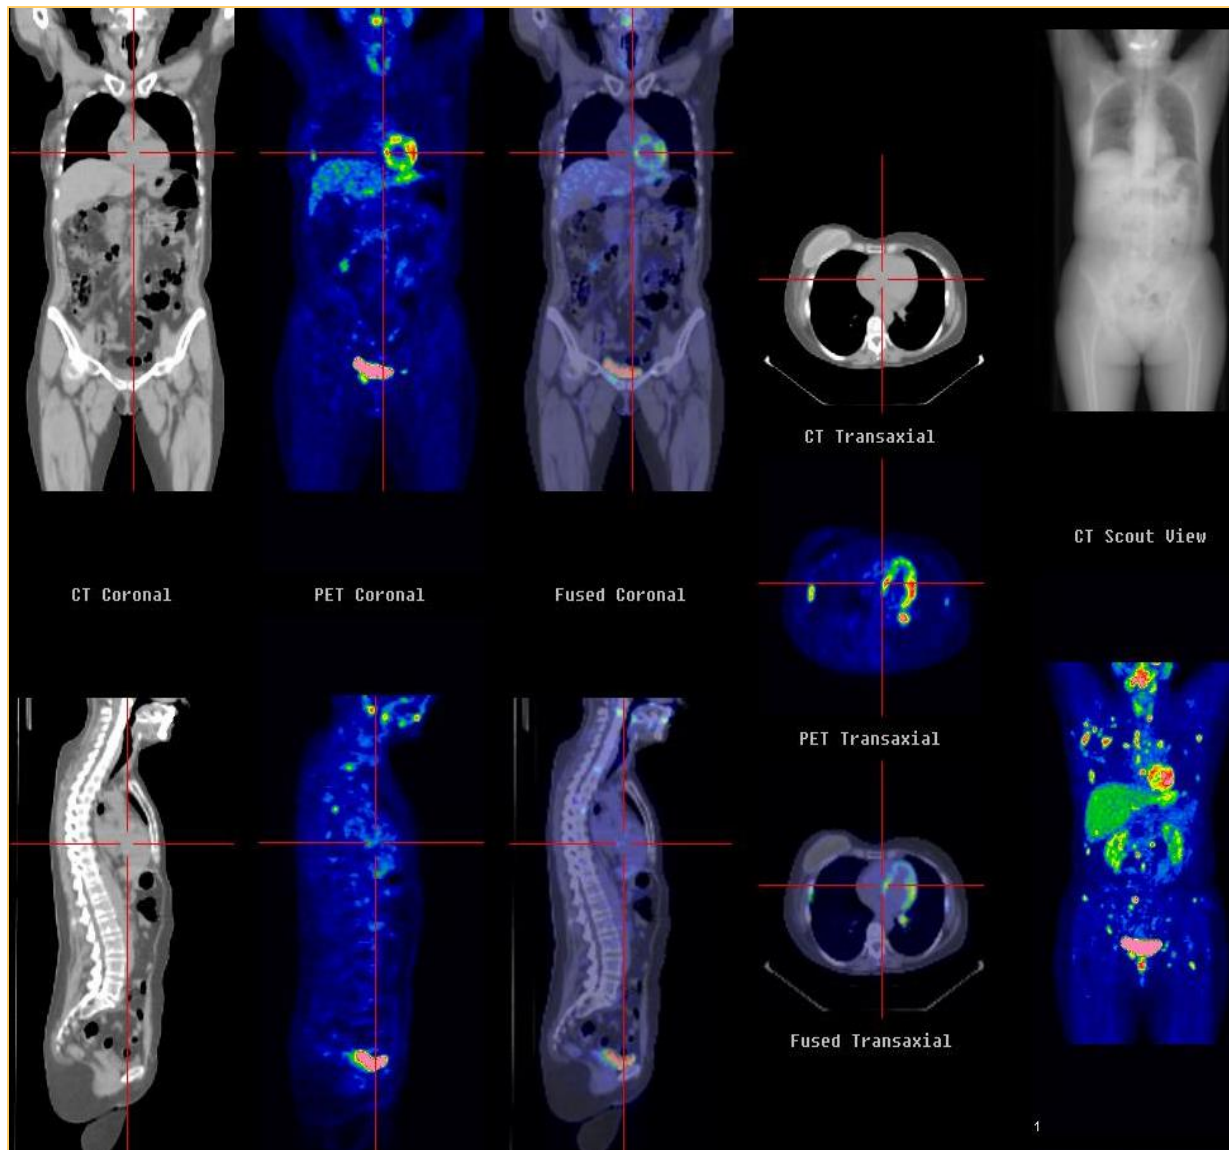

Courtesy HSR MILANO

The future of PET?

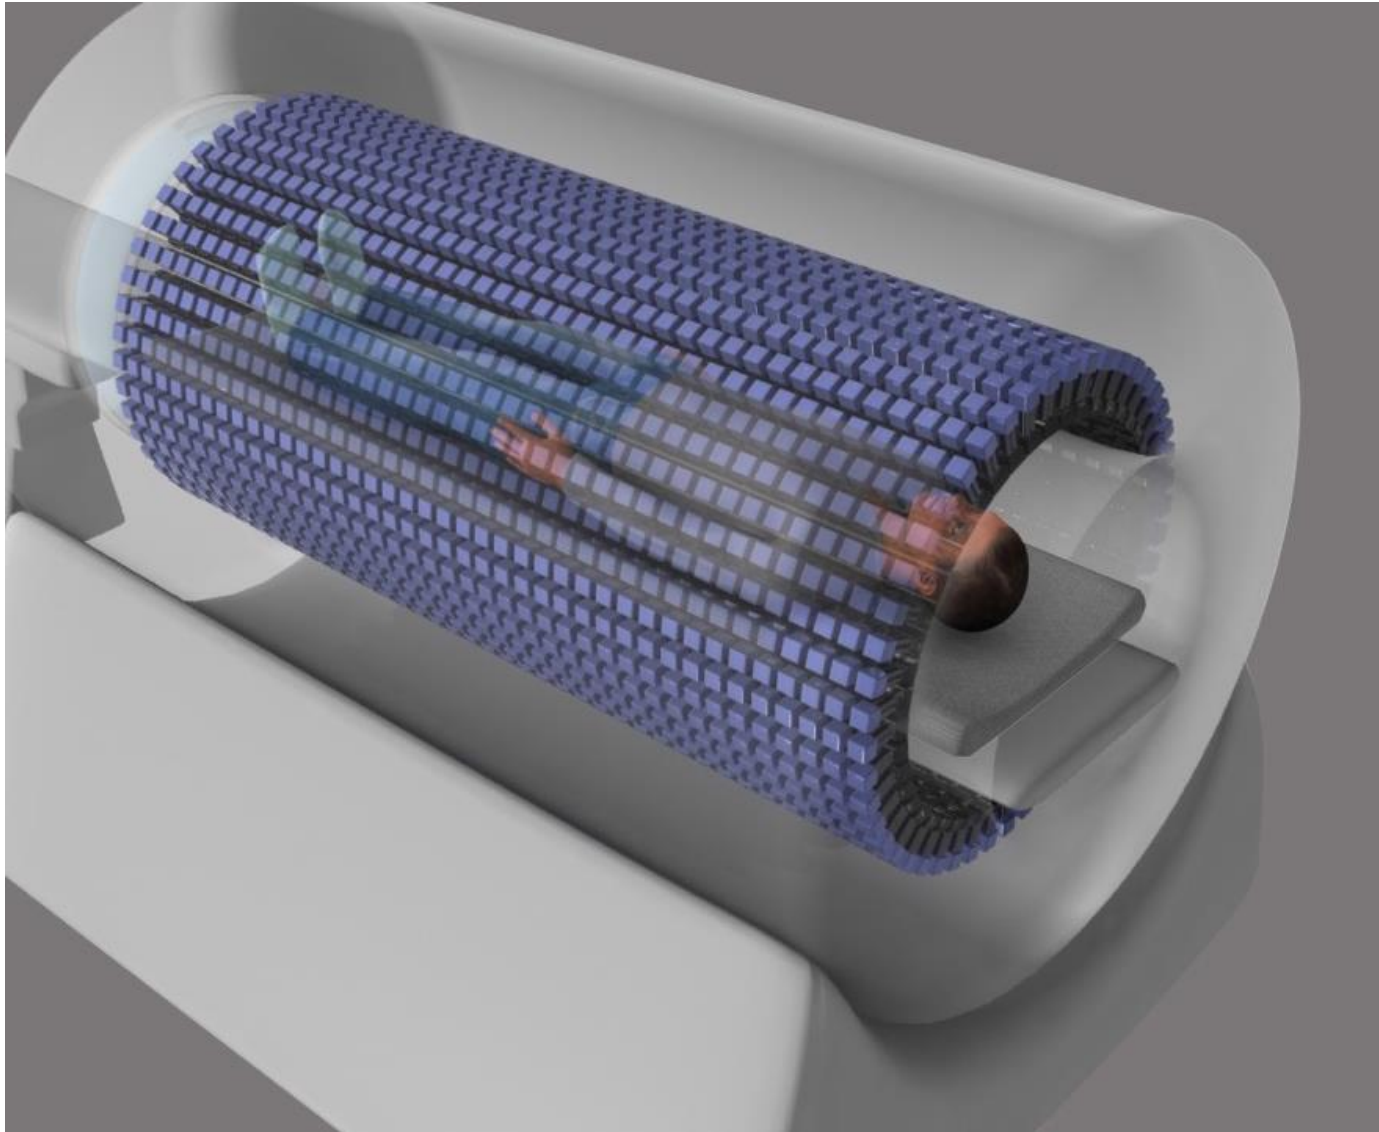

Outline of the lecture

Physics discoveries

Tools for physics applied to medicine

Medical imaging

X-ray CT

PET and PET/CT


Photon/electron radiation therapy

Hadron therapy

Three classes of medical accelerators


Electron linacs for conventional radiation therapy, including advanced modalities:

- Cyberknife
- IntraOperative RT (IORT)
- Intensity Modulated RT

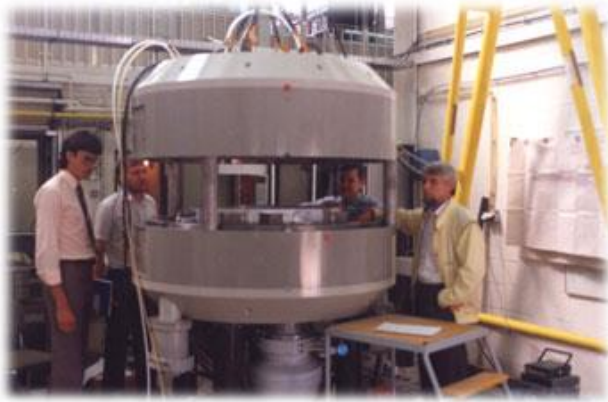


Low-energy cyclotrons for production of radionuclides for medical diagnostics



Medium-energy cyclotrons and synchrotrons for hadron therapy with protons (250 MeV) or light ion beams (400 MeV/u ^{12}C -ions)

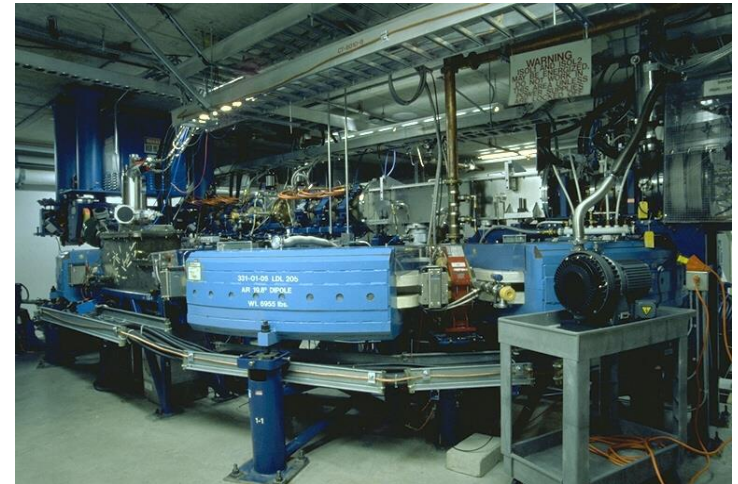


Availability of radiation therapy worldwide

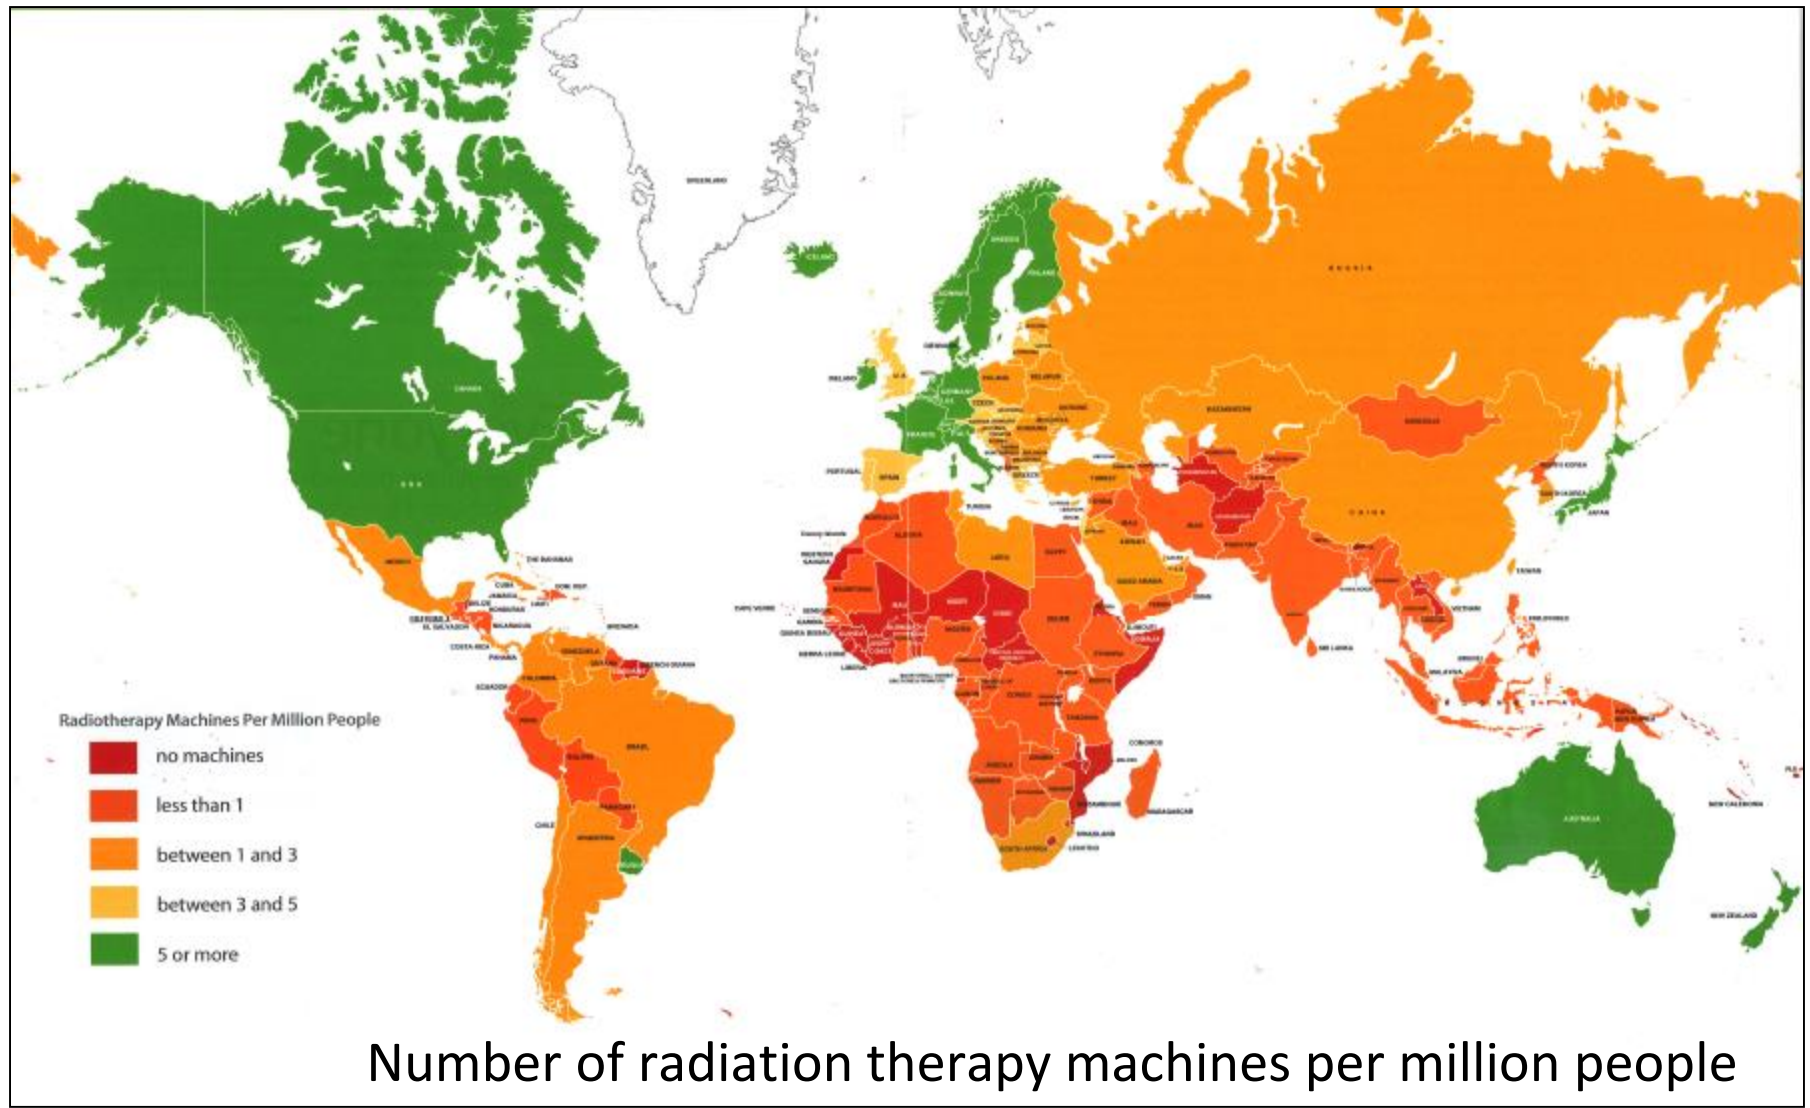



Treatment planning and dose delivery to tumour volume

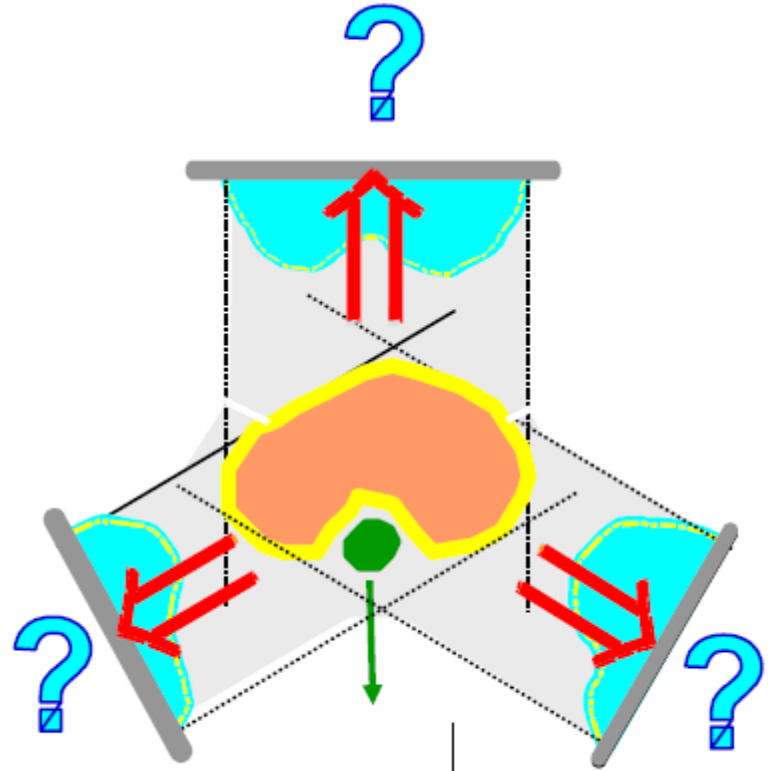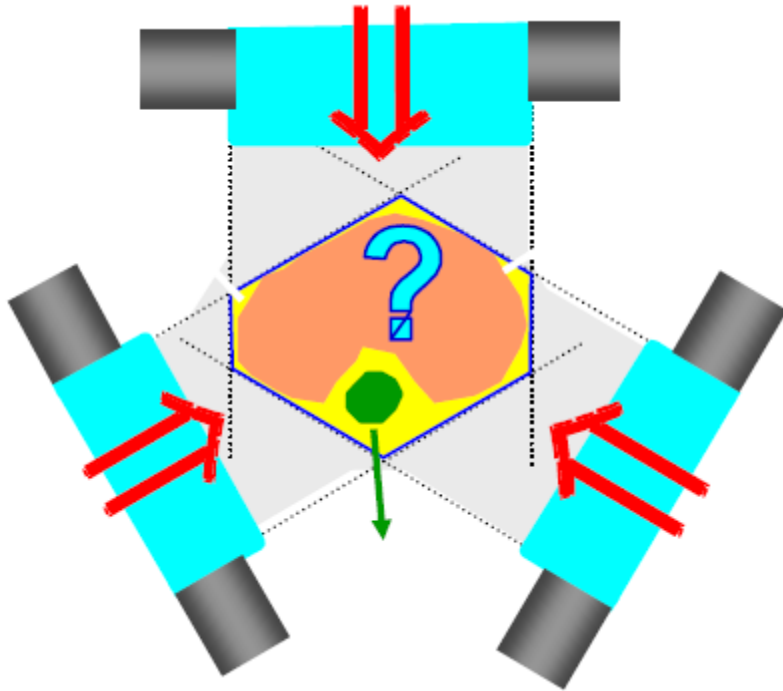


Tumour control and therapeutic window

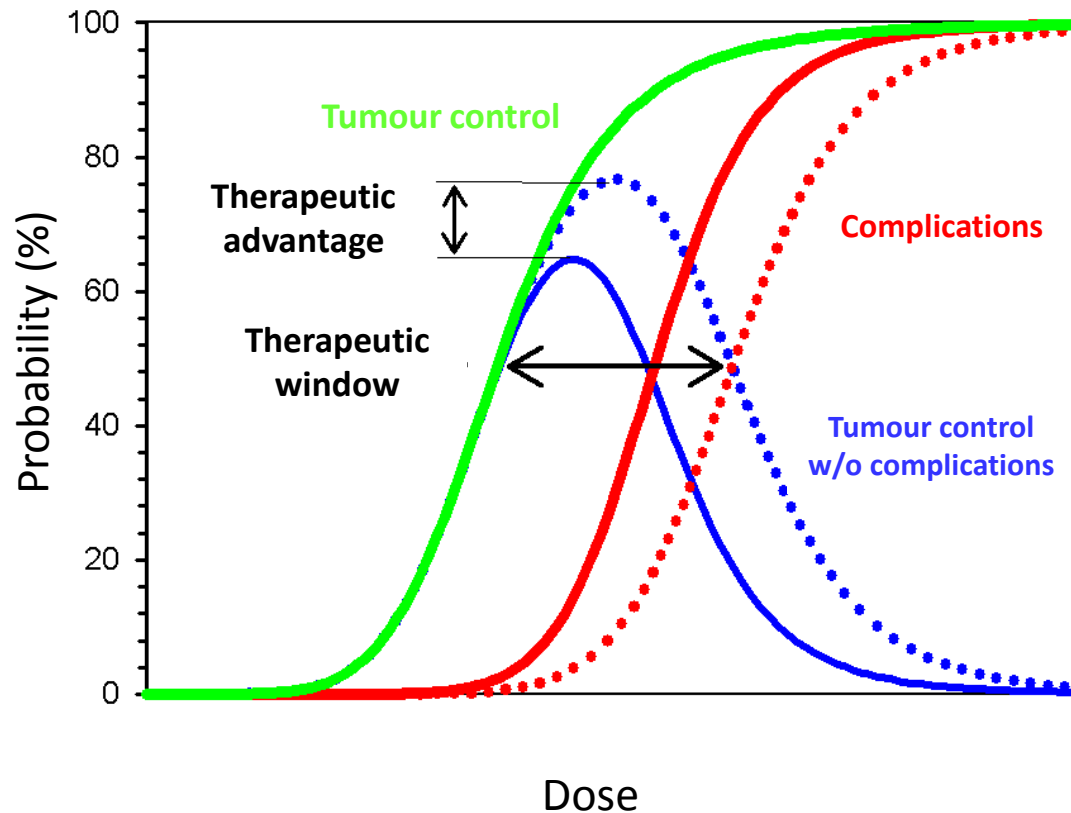

X-rays in radiation therapy: medical electron linacs

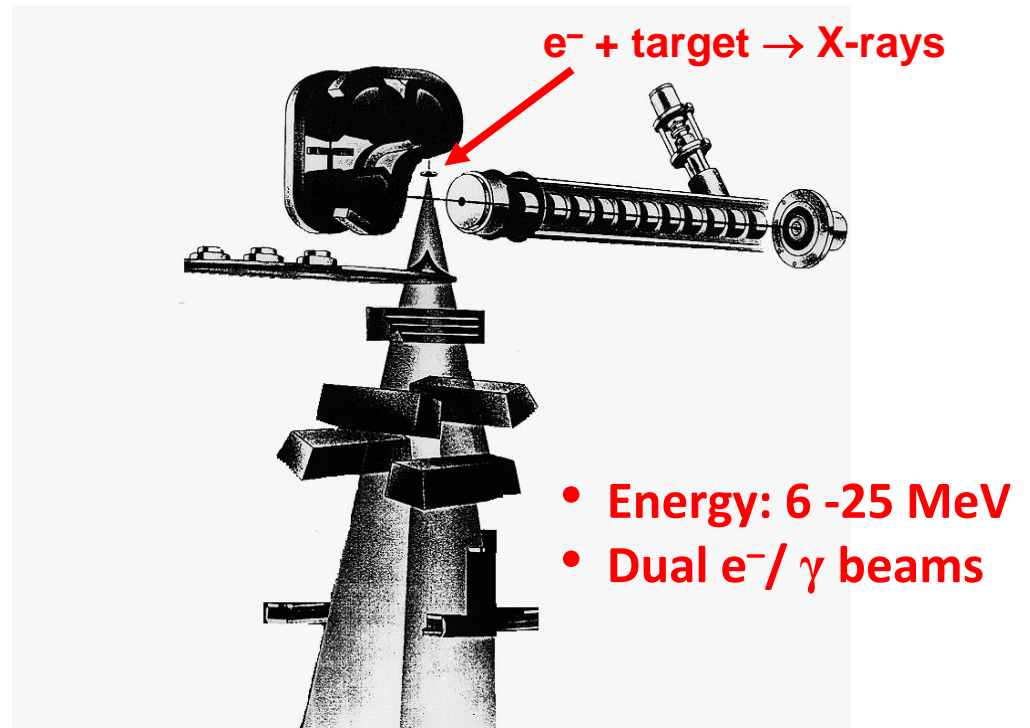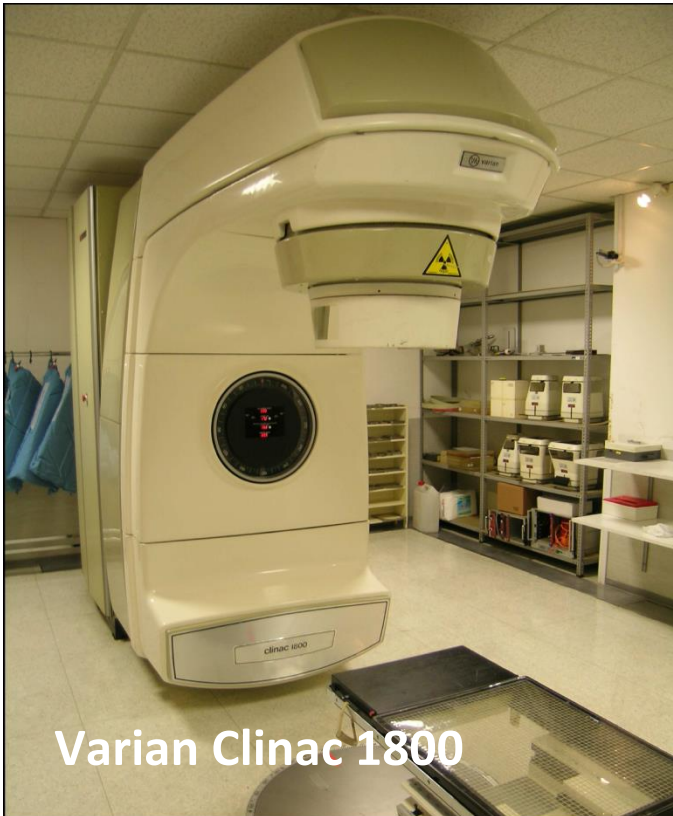

Multi-leaf collimator

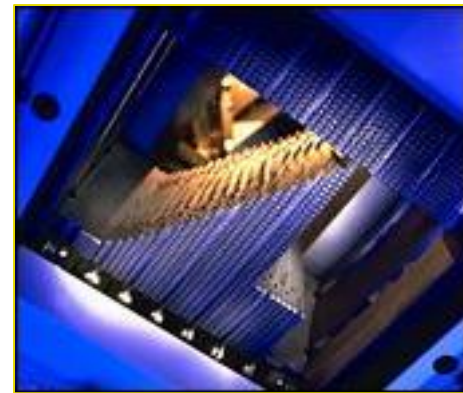

Intra-Operative Radiation Therapy (IORT)



- Small electron linac
- Energy 6 – 12 MeV
- Treatment with electrons only
- Single irradiation
- Three models of linac produced by three manufacturers (two in Italy)



CyberKnife (CK) Robotic Surgery System


6 MV Linac mounted on a robotic arm



- Non-Isocentric
- Average dose delivered per session is 12.5 Gy
- 6 sessions/day
- Dose rate @ 80 cm = 400 cGy/min

<http://www.accuray.com/Products/Cyberknife/index.aspx>

Intensity Modulated Radiation Therapy

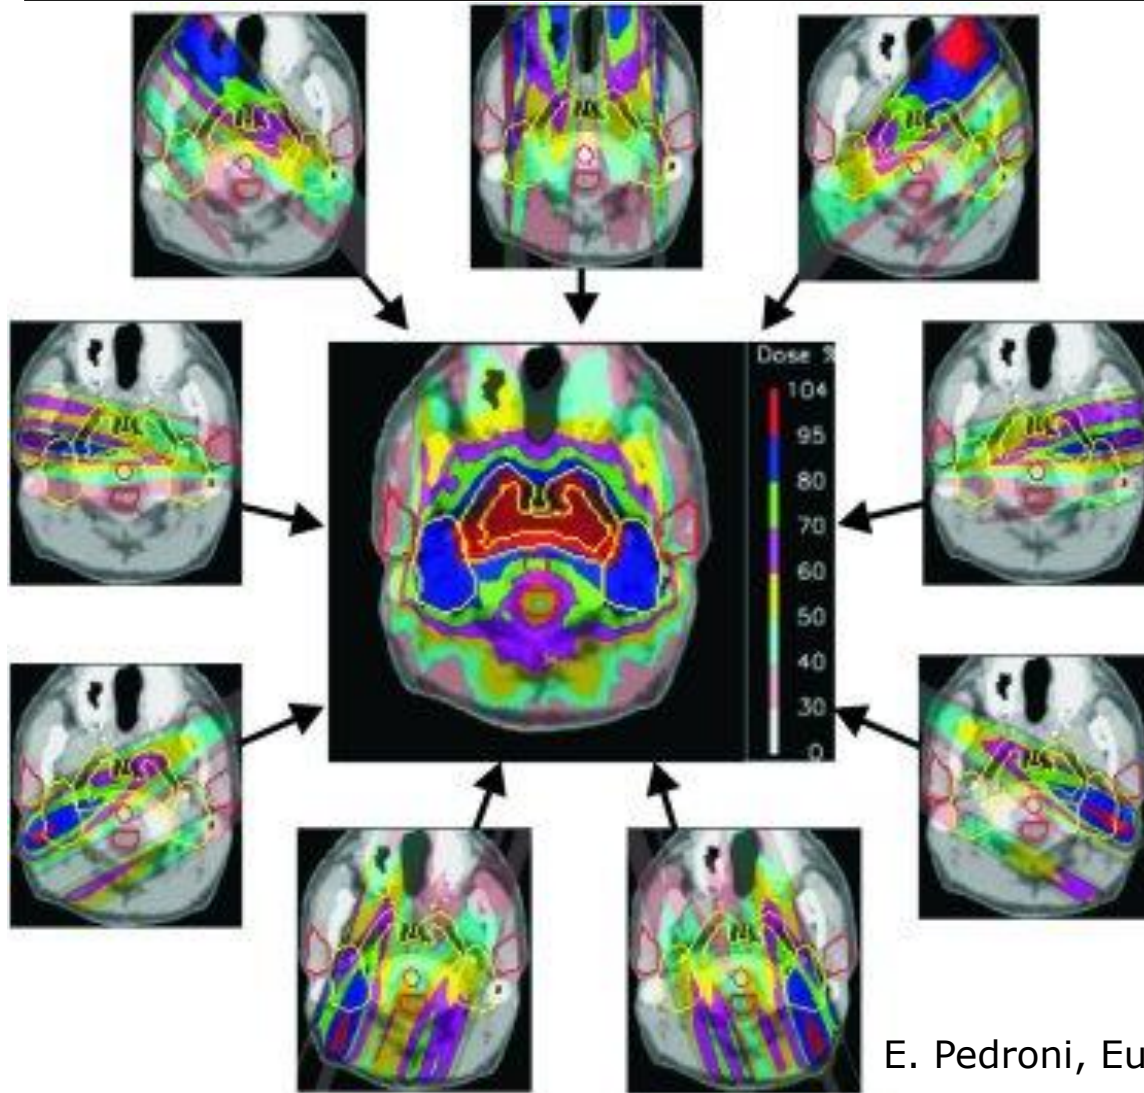


An example of intensity modulated treatment planning with photons. Through the addition of 9 fields it is possible to construct a highly conformal dose distribution with good dose sparing in the region of the brain stem (courtesy of T. Lomax, PSI).


E. Pedroni, Europhysics News (2000) Vol. 31 No. 6

Yet X-rays have a comparatively poor energy deposition as compared to protons and carbon ions

Helical tomotherapy

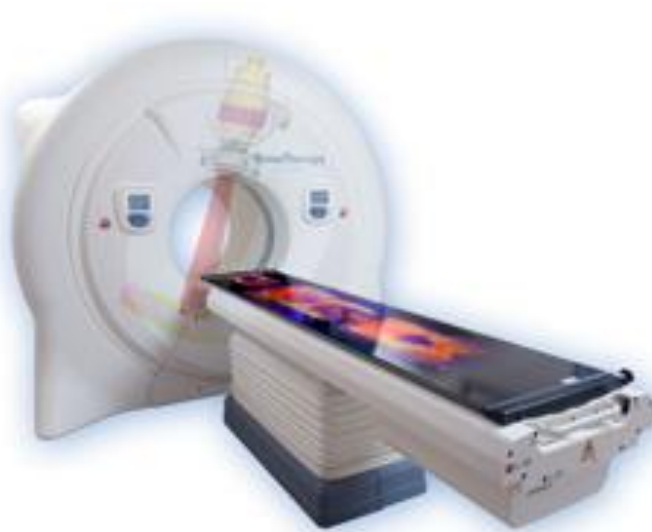


www.tomotherapy.com

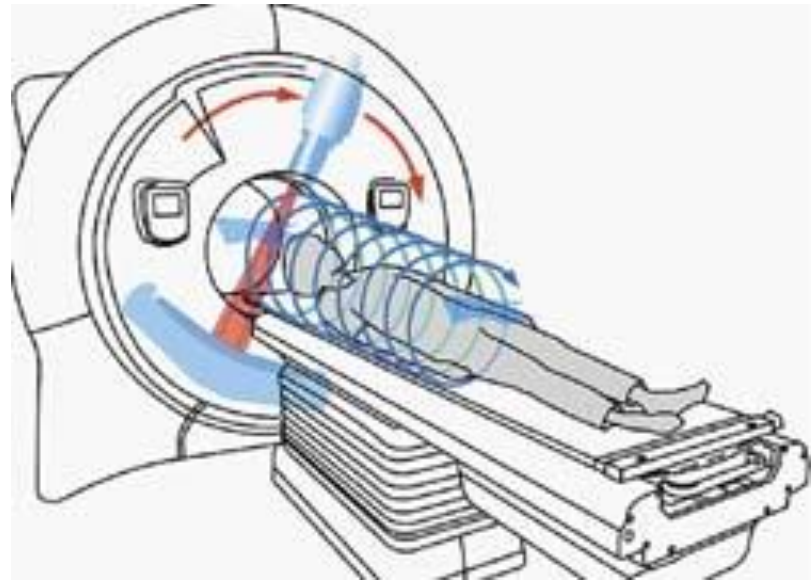

- **Integrated CT guidance**
 - Integrated CT scanner allowing efficient 3D CT imaging for ensuring the accuracy of treatment
- **A binary multi-leaf collimator (MLC)** for beam shaping and modulation
- **A ring gantry design** enabling TomoHelical delivery
 - As the ring gantry rotates in simultaneous motion to the couch, **helical fan-beam IMRT** is continuously delivered from all angles around the patient
- Very large volumes can be treated in a single set-up


Dedicated sequences for MRI guided radiotherapy treatments

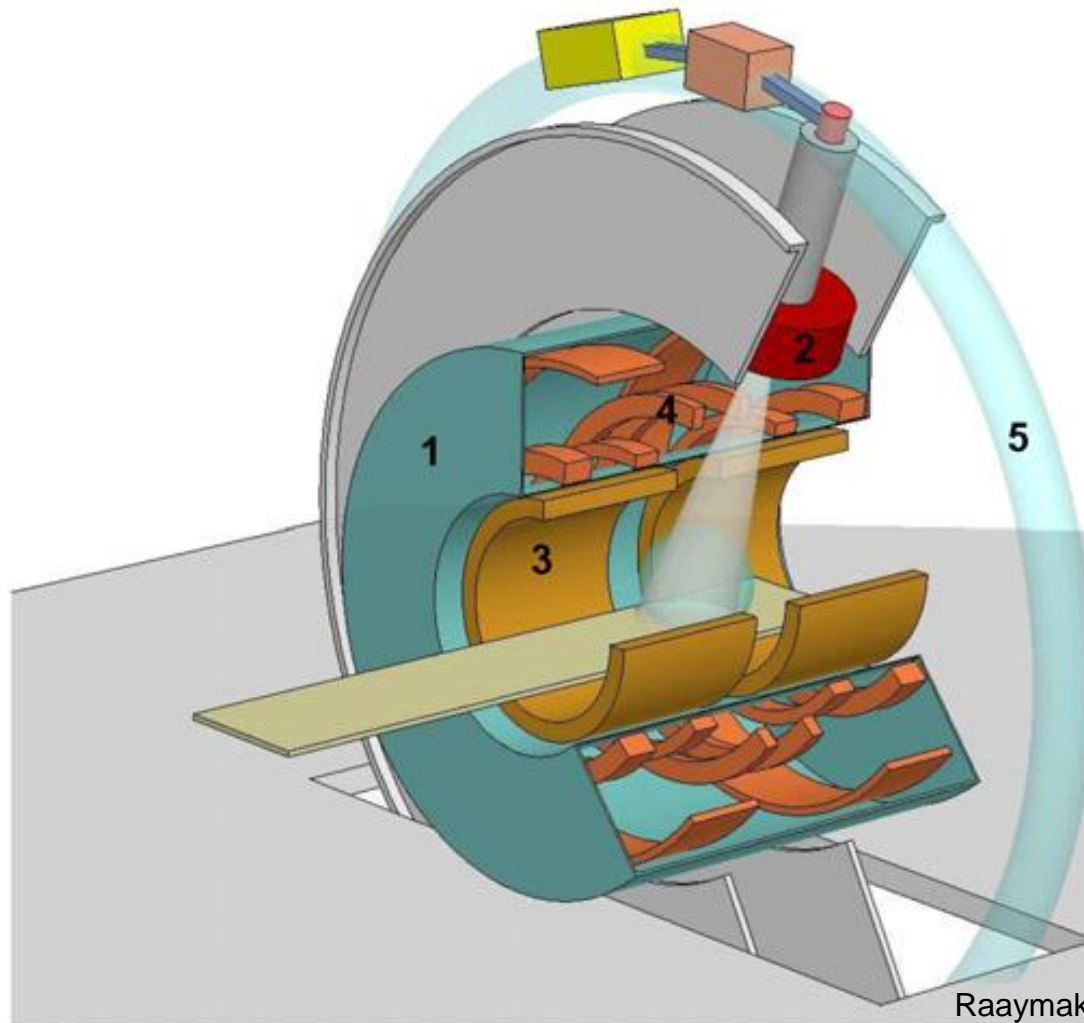


- 1) 1.5 T MRI
- 2) 6 MV accelerator
- 3) Split gradient coil
- 4) Superconducting coils
- 5) Low magnetic field toroid

Raaymakers et al, Phys. Med. Biol. **54** (2009) N229–N237


Hadrontherapy: n, p and C-ion beams

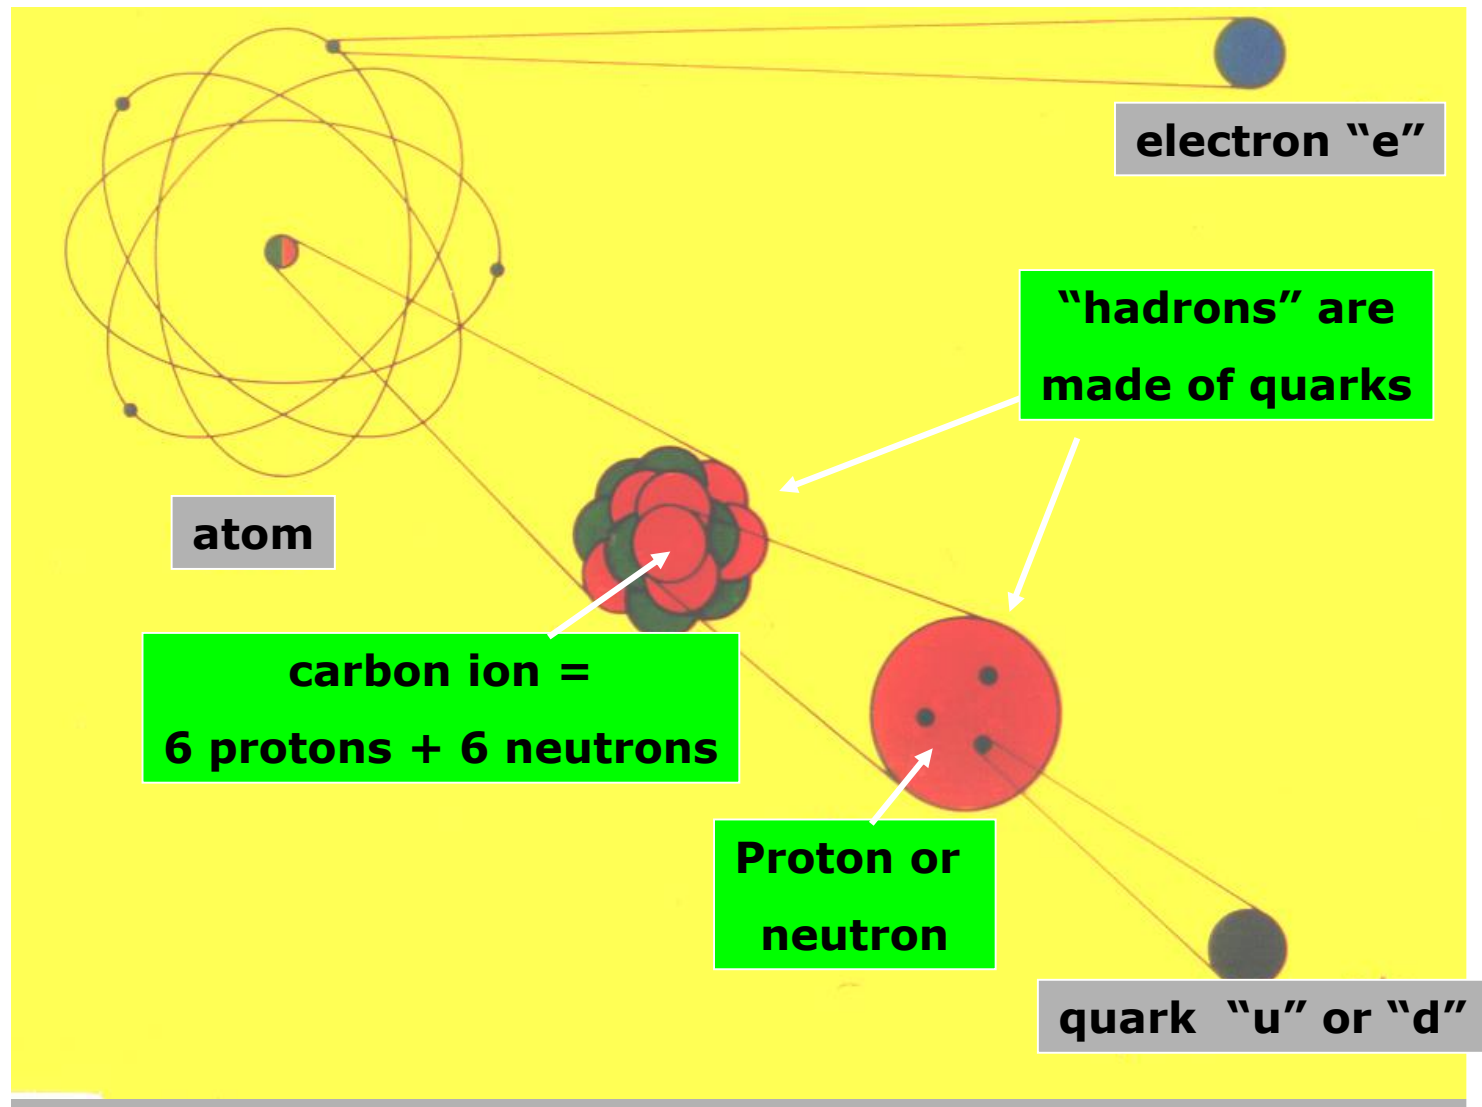


Proton radiation therapy

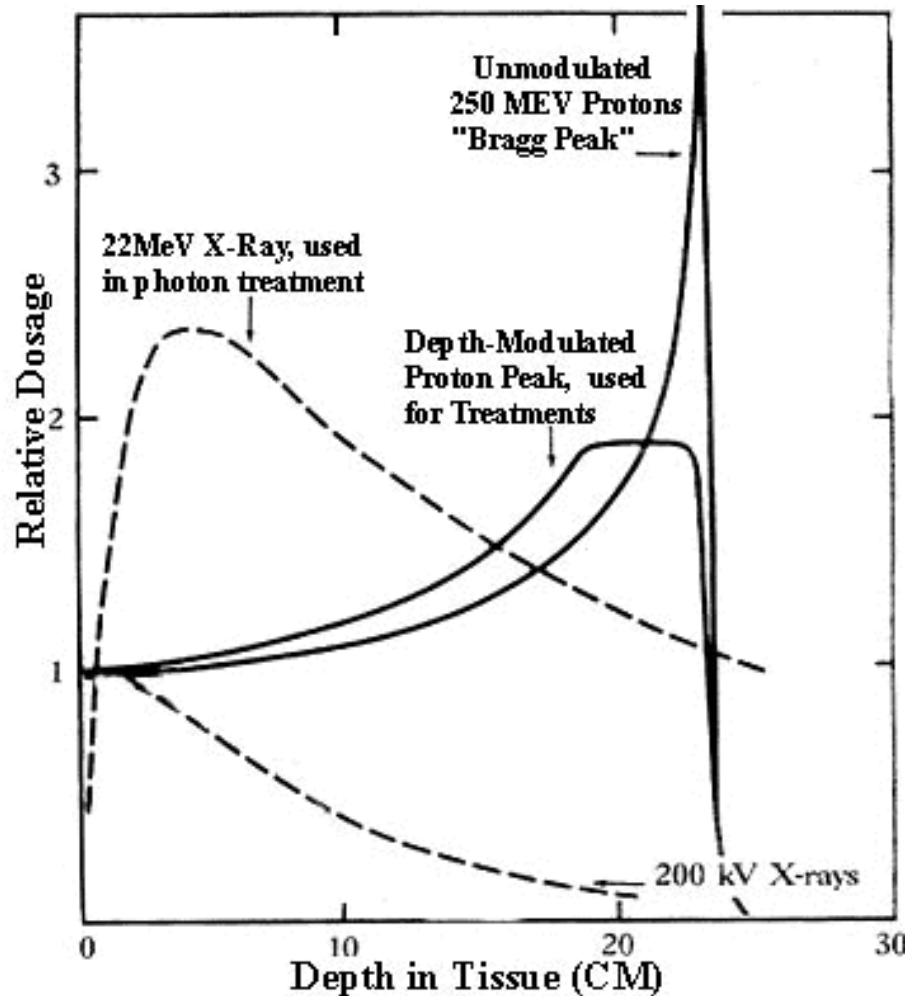


Prostate Cancer Treatment from the front.

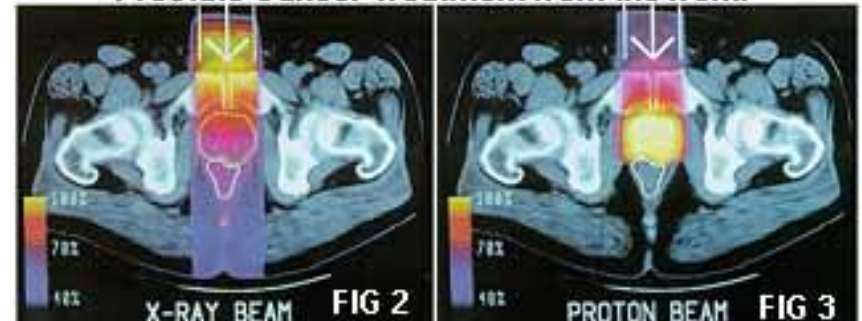

Prostate cancer treatment from the sides

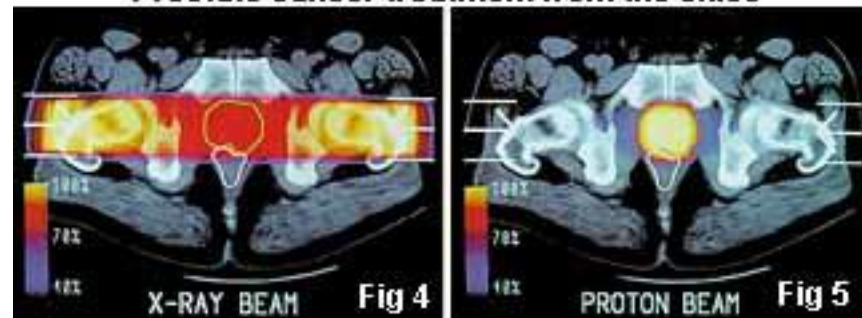


X-Ray vs Proton Side effects Treating Prostate cancer

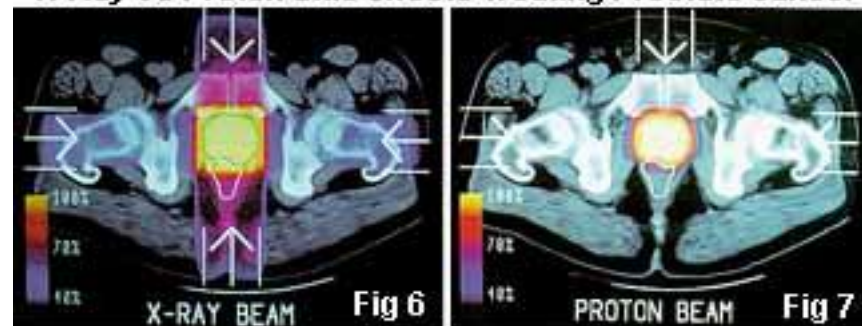


Treatment planning


- *Ion beam therapy is more conformal than photon beam RT*
- *Sharper dose fall off*
- *Range of ions much more influenced by tissue heterogeneities than photon beams with direct impact on TCP and NTCP*
- *Image guidance is necessary for ion beam therapy*

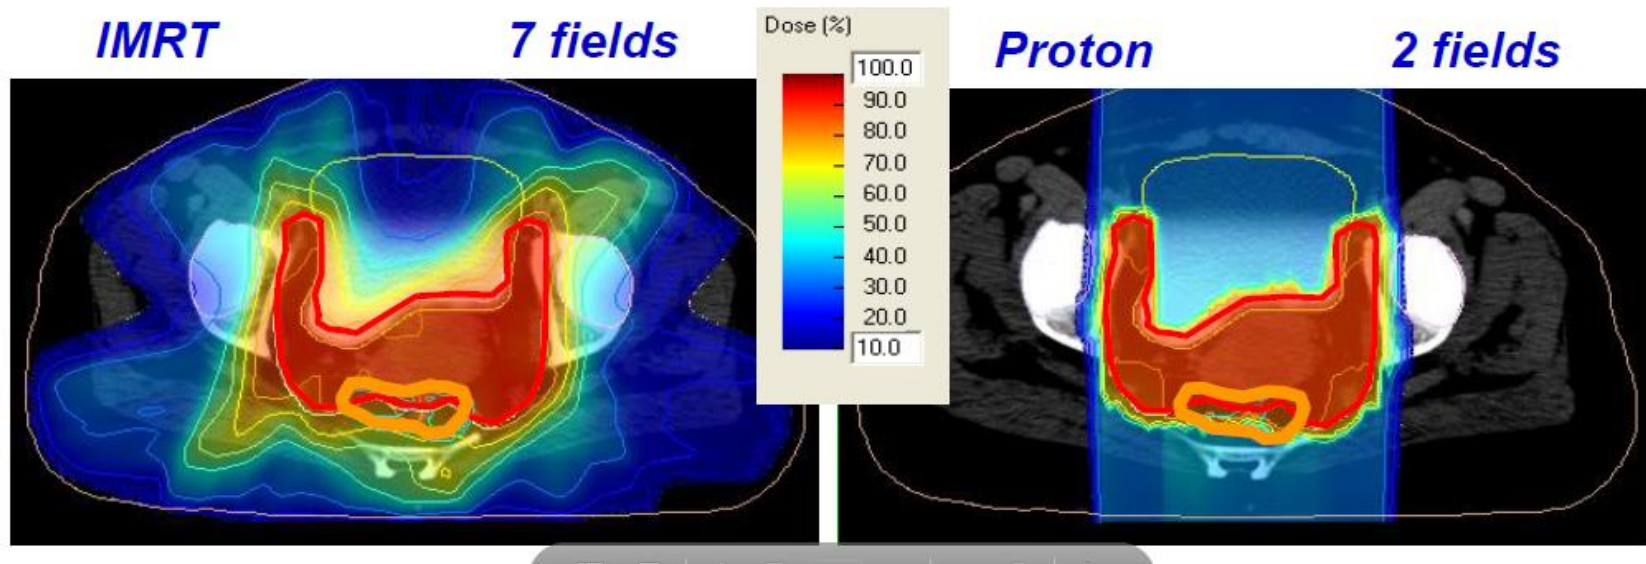

Radiobiological effectiveness (RBE)

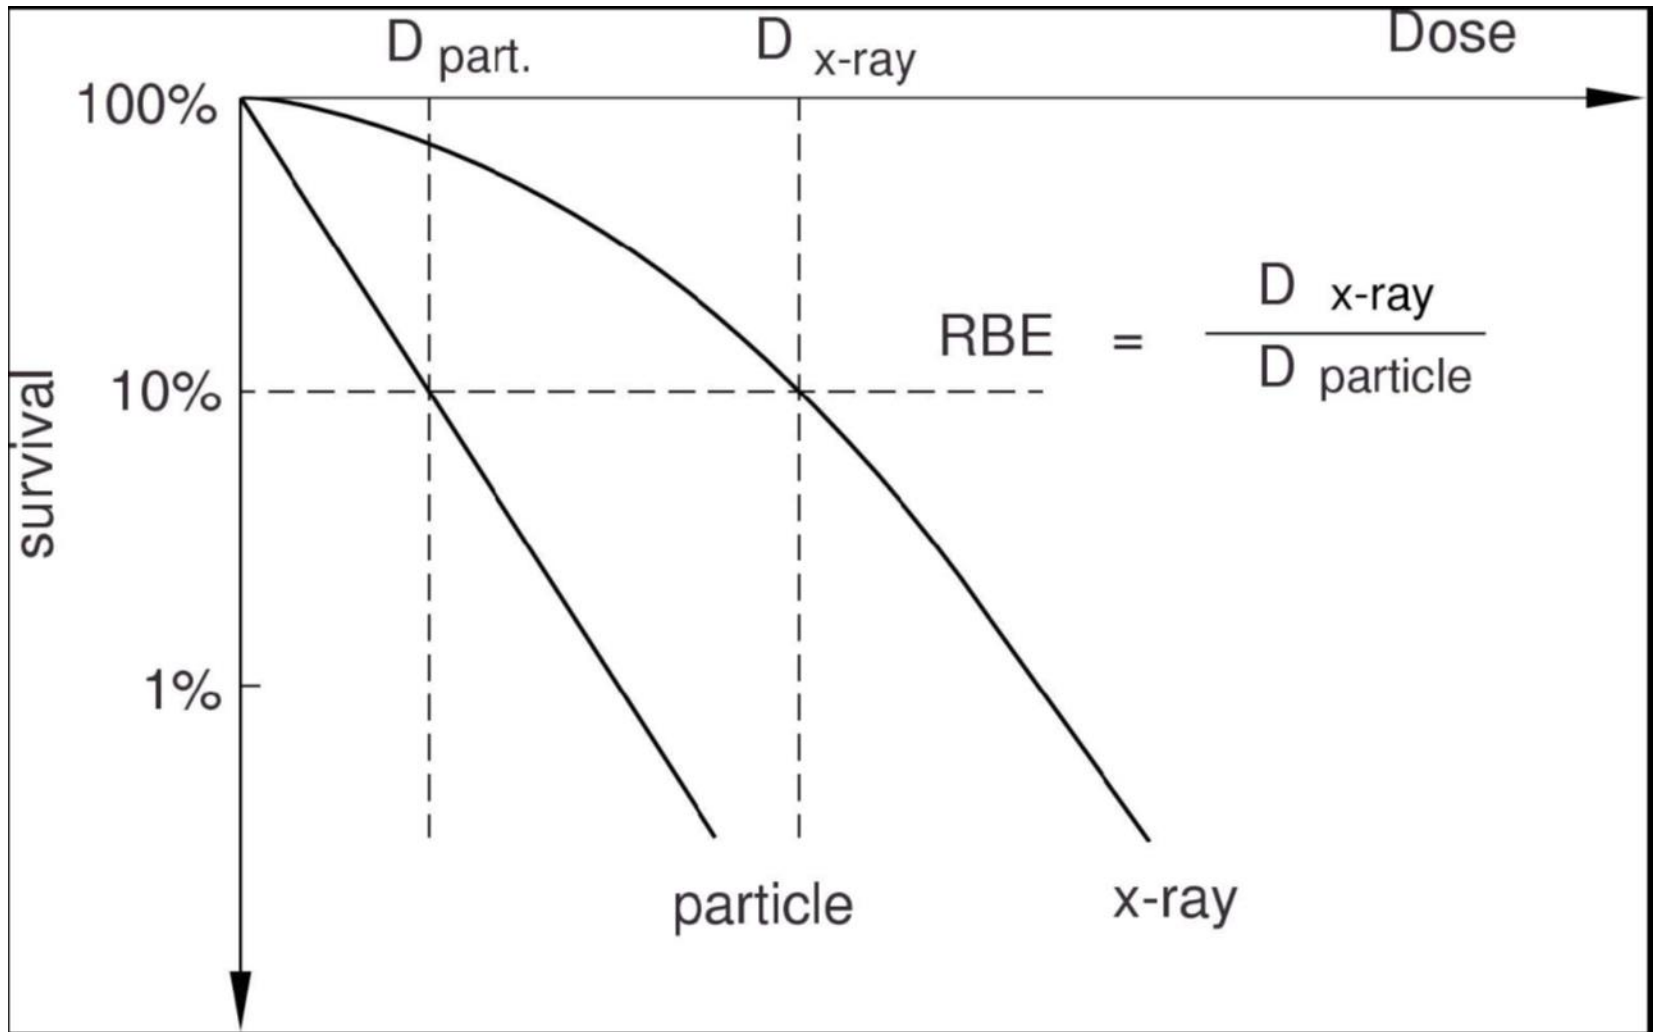

Hadrontherapy

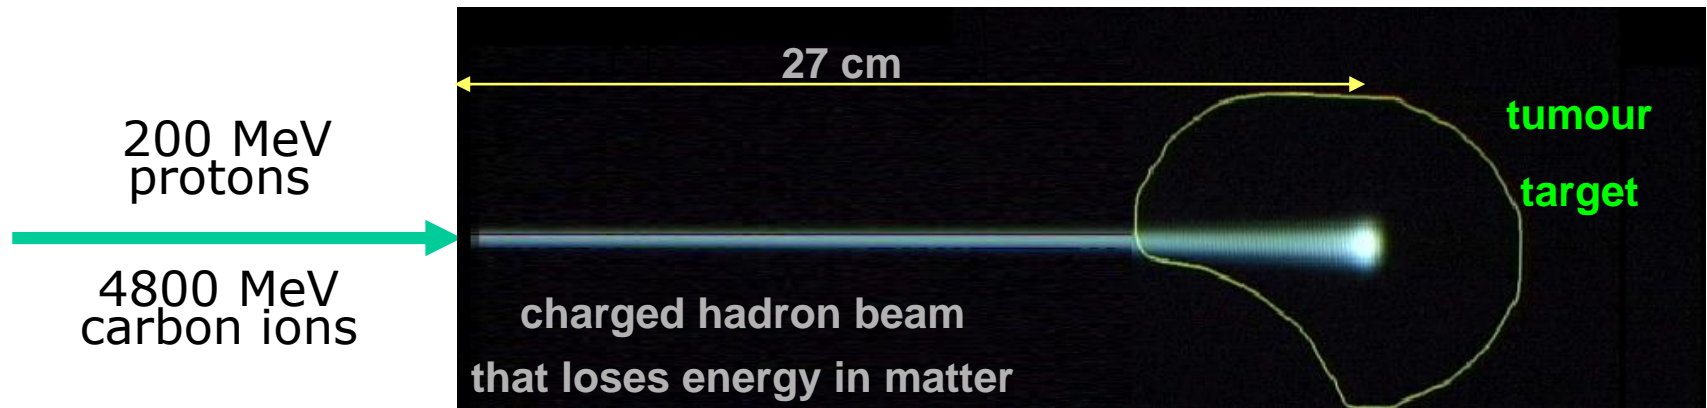


As of August 2015: 55 particle therapy facilities operation worldwide (mostly protons), 36 under construction, 14 at the planning stage

Number of patient treated until end of 2013


2054	He ions
1100	pions
13119	Carbon ions
433	other ions
105743	protons
122449	Grand Total

Proton radiation therapy

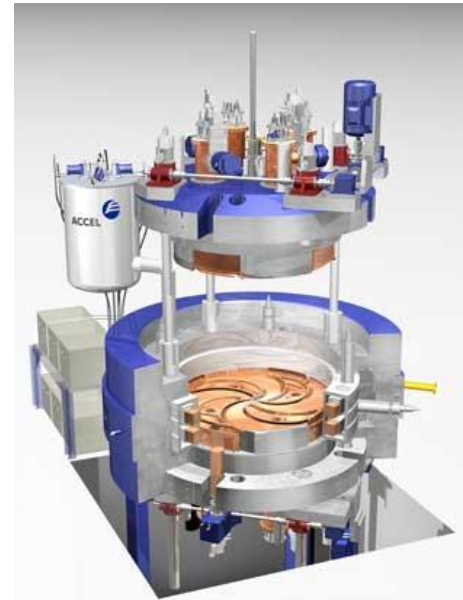


Accel-Varian


**Loma Linda
(built by FNAL)**

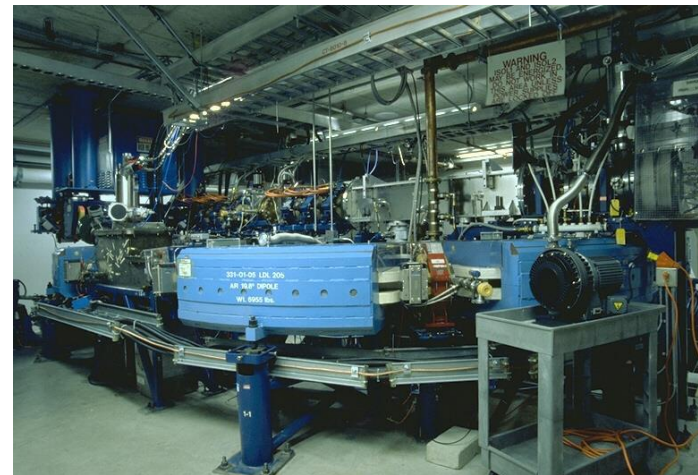


Loma Linda University Medical Center (LLUMC)

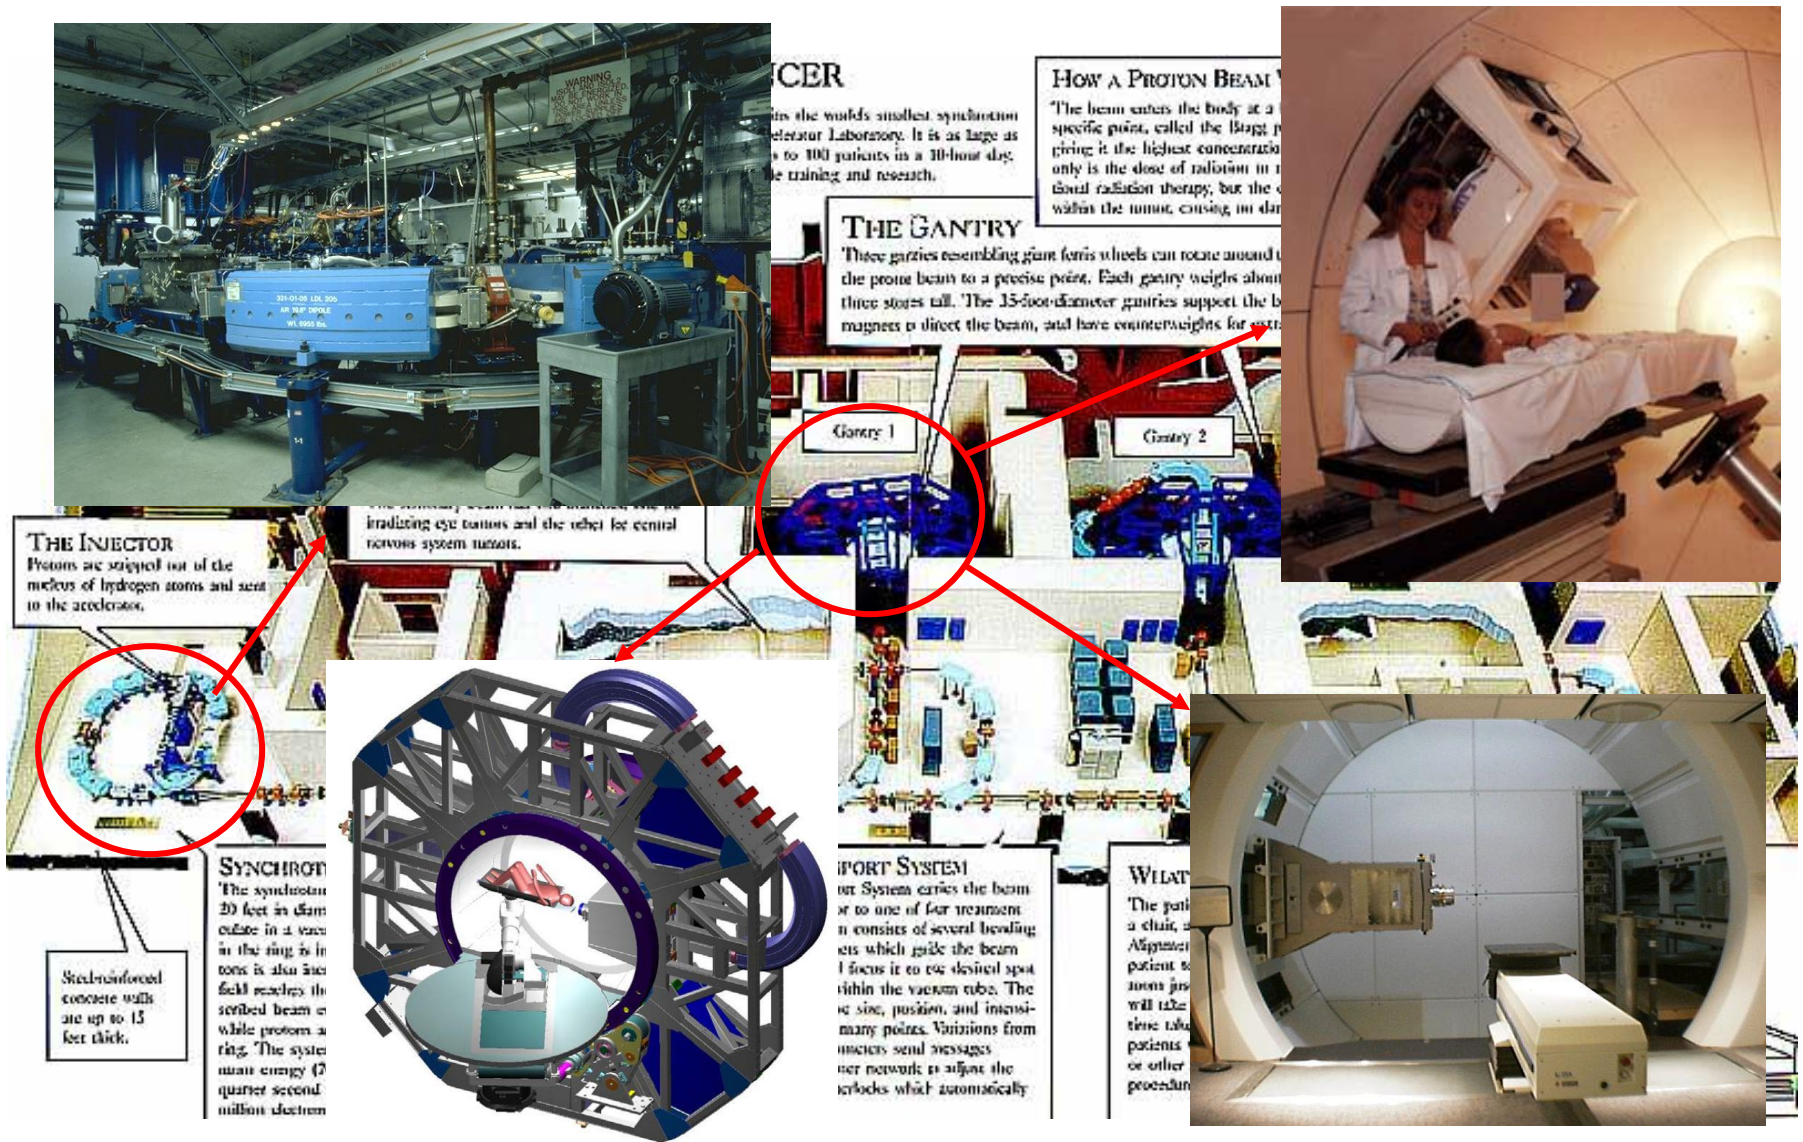

National Centre for Oncological Hadrontherapy, CNAO, Pavia, Italy

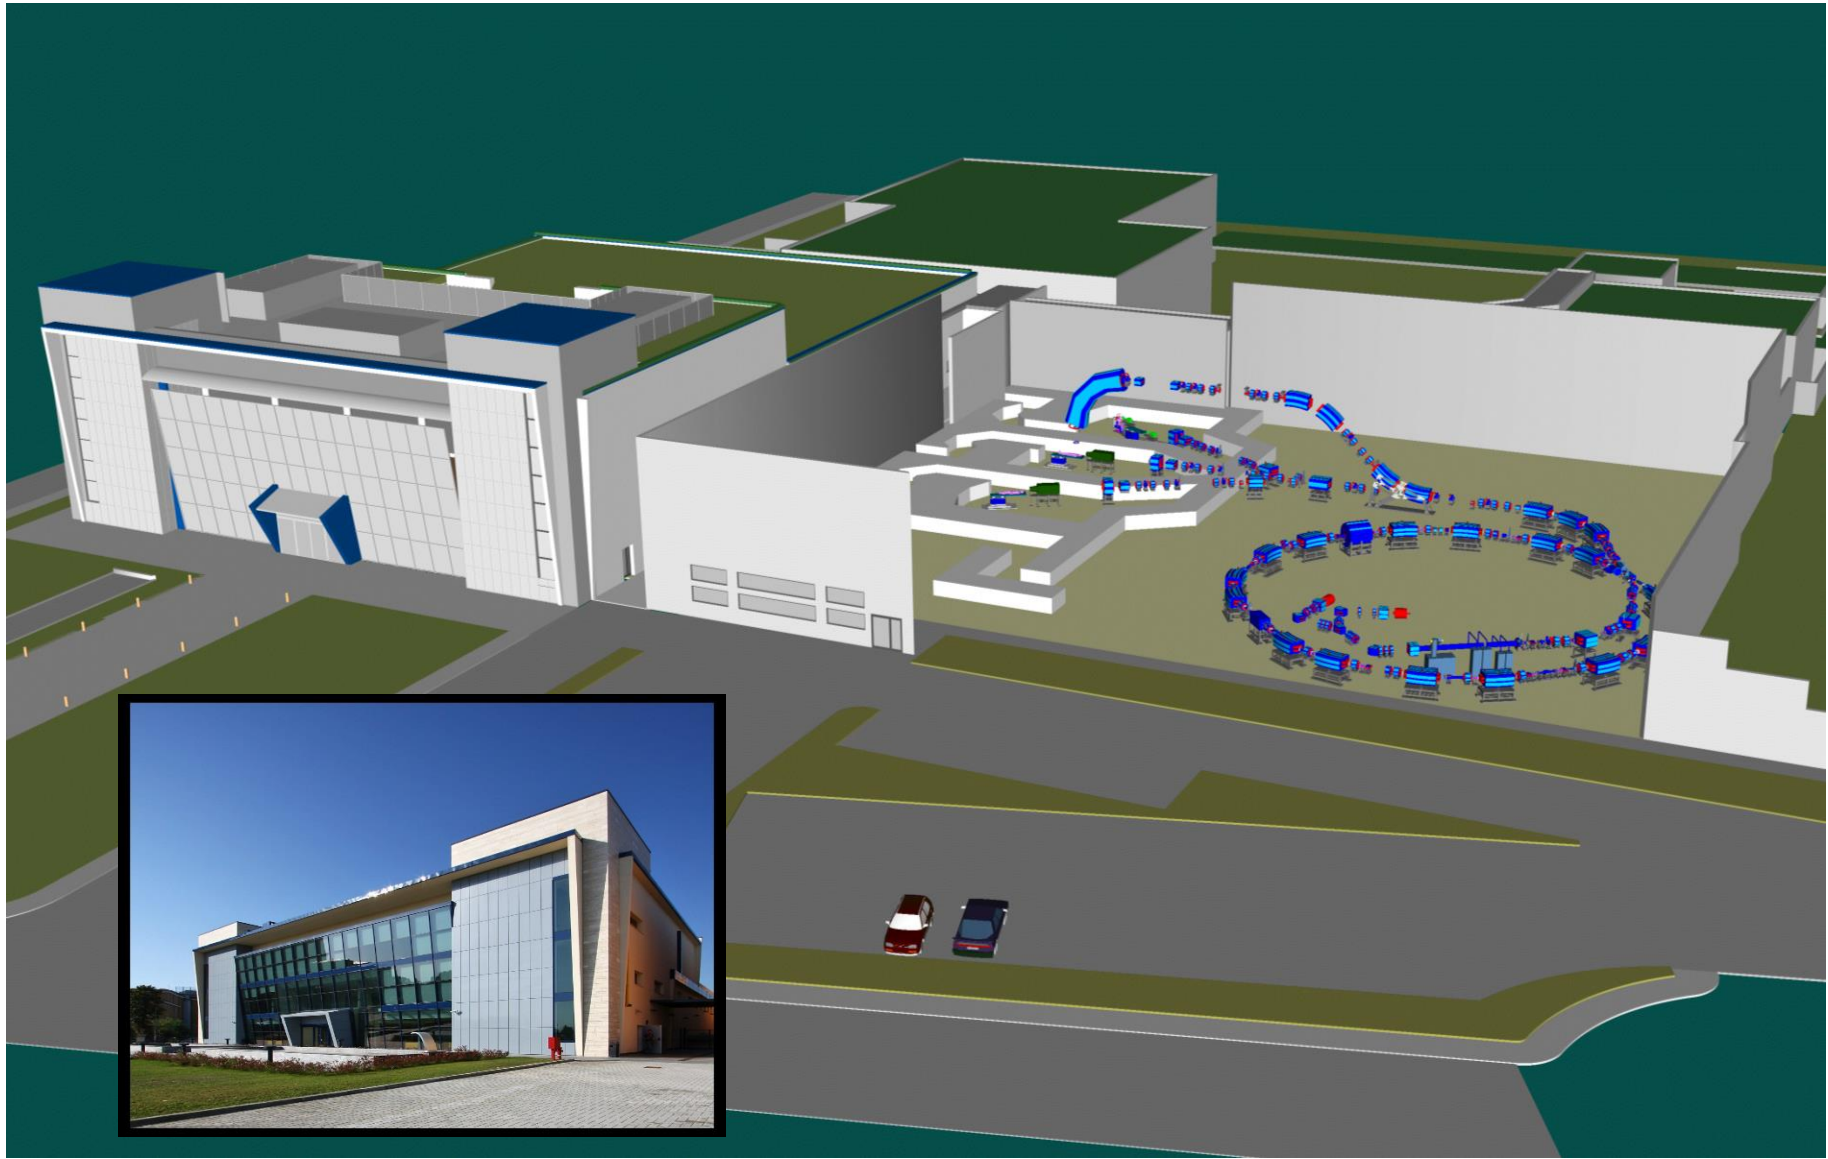


National Centre for Oncological Hadrontherapy, CNAO, Pavia, Italy

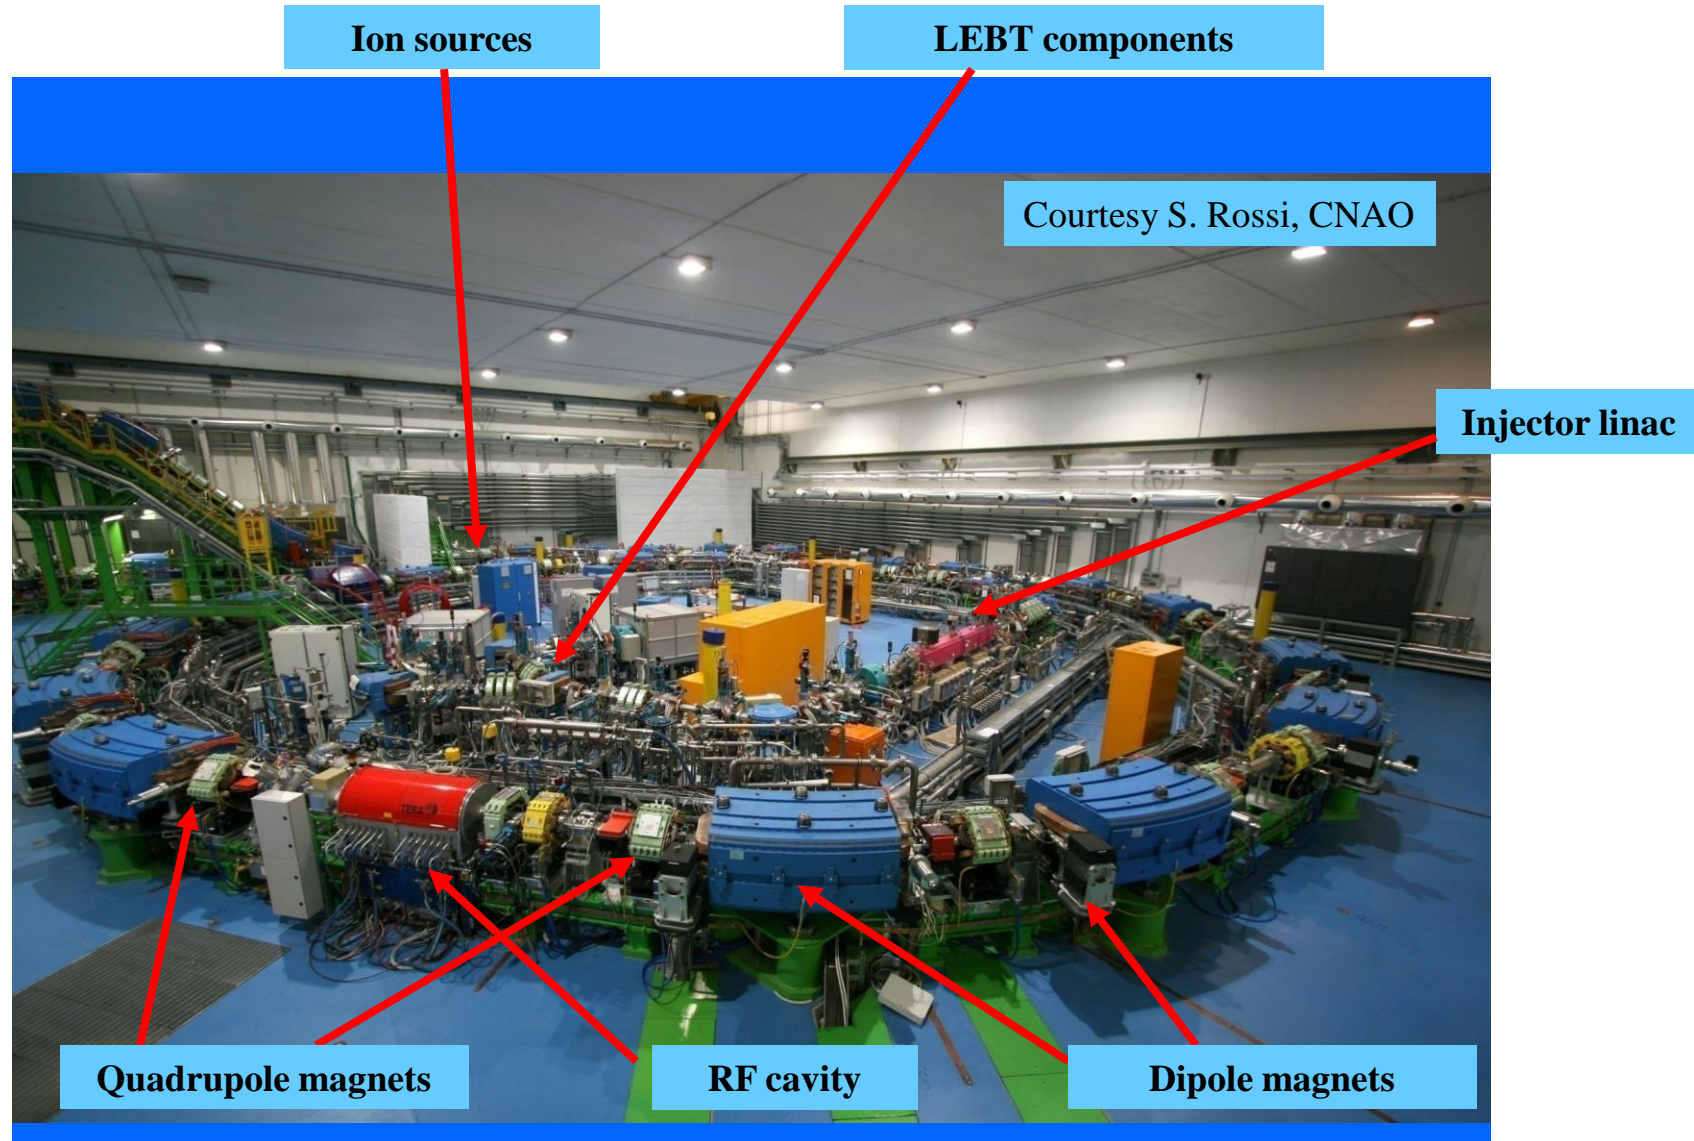




The future of hadrontherapy: single room facilities ?

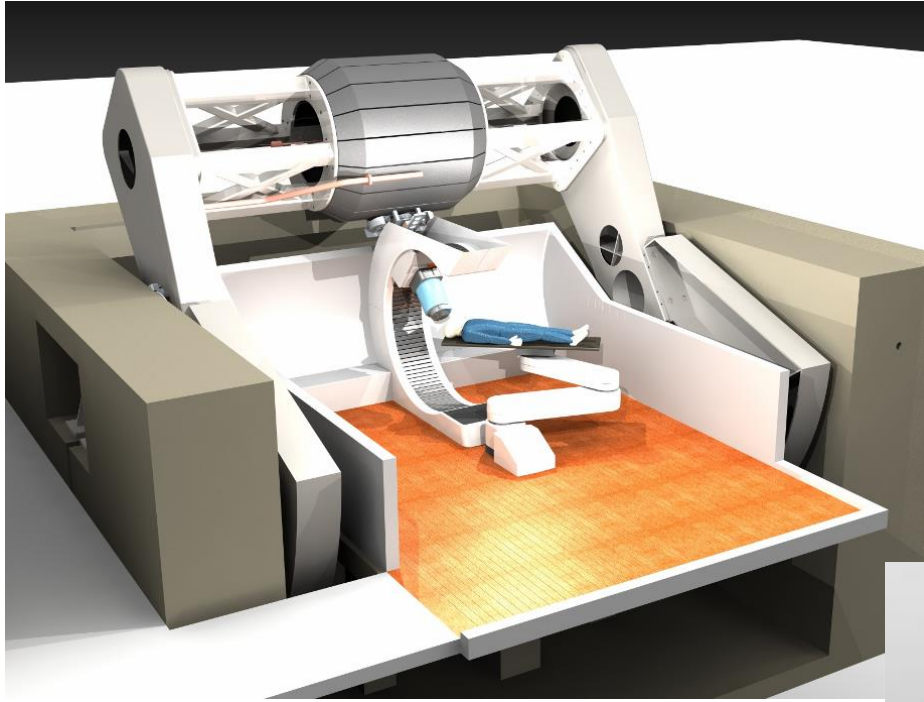

IBA Proteus Nano

Mevion Medical Systems

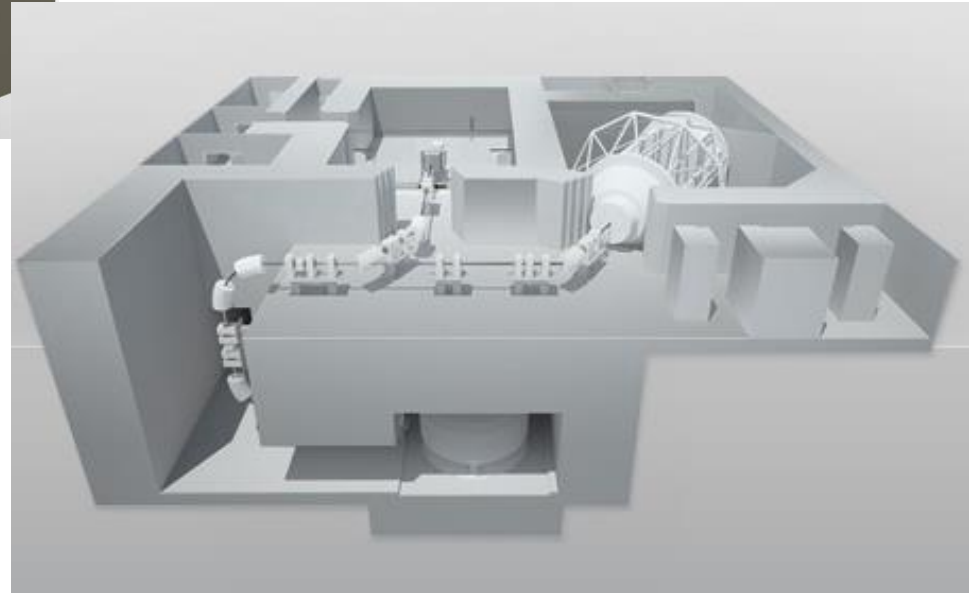

Acknowledgements

I am indebted to Prof. Ugo Amaldi (TERA Foundation and University of Milano Bicocca, Italy) and Prof. Maria Carla Gilardi (University of Milano Bicocca, Italy) for providing me with some of the slides that I have shown you today.