



Universität
Zürich ^{UZH}



elusive
neutrinos, dark matter & dark energy physics



Energy calibration for the GERDA experiment

C. Ransom

Zurich PhD seminar 2018

9 March 2018

Outline



- Detecting neutrinoless double-beta decay ($0\nu\beta\beta$)
- GERDA and the calibration procedure
- Energy scale calibration and stability
- Determining resolution at $Q_{\beta\beta}$
- Future developments
- Conclusion

Detecting $0\nu\beta\beta$

- Can explain mass of neutrino with small Majorana mass component
- Allows for $0\nu\beta\beta$ decay: hypothetical lepton number violating process
- Signature would be monoenergetic line, $Q_{\beta\beta}$, in energy spectrum of emitted electrons, 2039 keV for ^{76}Ge
- Sensitivity to half-life of decay:


$$T_{1/2}^{0\nu} \propto \epsilon \sqrt{\frac{Mt}{BI \cdot \Delta E}}$$

where ϵ : efficiency; Mt : exposure;
 BI : background events per kg·yr·keV;
 ΔE : resolution





GERDA and the calibration procedure

- Knowledge of energy scale, resolution vital for all physics analyses
- Detectors calibrated by ^{228}Th sources ea. 7-10 days
- Three sources lowered to three positions from above cryostat for $\approx 2\text{h}$
→ all detectors exposed
- Source Insertion System (SIS) built in Zurich
 - Operating reliably since 2011
 - Two independent measurement systems determine position of source to $\pm 1\text{ mm}$



GERDA and the calibration procedure (cont.)

- 40 detectors, two main types:
Semi-coaxial (Coax) and Broad Energy Germanium (BEGe)
- Germanium detectors have excellent resolution (~ 3 keV for BEGe, ~ 4 keV for Coax)





Coax




BEGe

Energy scale calibration

- GERDA calibration software identifies, fits peaks in spectra for each detector
- Calibration curves are linear fit between reconstructed and physical energy
- Range of peaks fitted between 583 keV and 2.6 MeV



Calibrated energy: 860 keV




Detector: GD91A, Date: 20180224


Stability monitoring

- Energy scale stability required for combining of data between calibrations → stability should not limit resolution
- Stability of position, resolution of 2.6 MeV ^{228}Th peak monitored calibration to calibration
- Shifts of 2.6 MeV peak usually $\lesssim 0.5$ keV

Energy scale stability



Resolution stability




Resolution at $Q_{\beta\beta}$

- Recall:


$$T_{1/2}^{0\nu} \propto \epsilon \sqrt{\frac{Mt}{BI \cdot \Delta E}}$$

- Sensitivity depends strongly on resolution
- Poor resolution would leak to $2\nu\beta\beta$ events leaking towards $Q_{\beta\beta}$
- Want to know resolution at $Q_{\beta\beta}$ in physics spectrum
- Procedure:
 - Combine many calibration spectra for each detector
 - Fit peaks, find resolution at each peak
 - Combine resolutions for each dataset, weighting by exposure
 - Fit resolution curve, interpolate to $Q_{\beta\beta}$





Resolution at $Q_{\beta\beta}$ (cont.)

- Step 1: Combine calibration spectra for each detector
 - Easy! Simply add up all calibration spectra!



Resolution at $Q_{\beta\beta}$ (cont.)

- Step 1: Combine calibration spectra for each detector ✓
- Step 2: Fit peaks, find resolution at each peak
 - Easy! Use existing calibration software, apply to combined spectra.



Resolution at $Q_{\beta\beta}$ (cont.)

- Step 1: Combine calibration spectra for each detector ✓
- Step 2: Fit peaks, find resolution at each peak ✓
- Step 3: Combine resolutions for each dataset
 - Weight by exposure: how much a single detector contributes to physics spectrum for each dataset
 - Not so easy...

Resolution at $Q_{\beta\beta}$: Combining detector resolutions


- Combination of many Gaussians is a Gaussian mixture, so:

$$\sigma^2 = \sum_i w_i (\sigma_i^2 + \mu_i^2) - \sum_i (w_i \cdot \mu_i)^2$$

- Assume all means are equal (correctly calibrated peaks!):

$$\sigma^2 = \sum_i w_i \sigma_i^2$$

where \sum_i is sum over detectors, w_i is detector exposure, σ_i , μ_i are the resolutions / mean positions for each detector

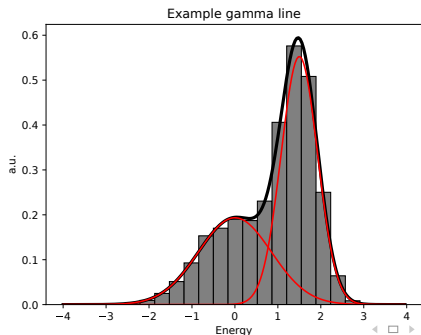


Resolution at $Q_{\beta\beta}$ (cont.)

- Step 1: Combine calibration spectra for each detector ✓
- Step 2: Fit peaks, find resolution at each peak ✓
- Step 3: Combine resolutions for each dataset, weighting by exposure
 - Use Gaussian mixture equation

Resolution at $Q_{\beta\beta}$ (cont.)

- Step 1: Combine calibration spectra for each detector ✓
- Step 2: Fit peaks, find resolution at each peak ✓
- Step 3: Combine resolutions for each dataset, weighting by exposure ✓
- Step 4: Fit resolution curve, interpolate to $Q_{\beta\beta}$
 - Empirically, fit equation: $\text{FWHM}(E) = \sqrt{aE + b}$
 - Doppler broadened single-escape peak is excluded




At $Q_{\beta\beta} = 2039$ keV

Coax FWHM:
 3.55 ± 0.02 keV

BEGe FWHM:
 2.94 ± 0.01 keV

Future developments

- Current method of simply adding spectra is not perfectly representative of physics data
 - Some calibrations are longer than others, exposure is not identical for each calibration
 - Calibrations are not applied for the same period of time
- New method (in development)



Future developments (cont.)

- Some complications:
- Not trivial to normalise
 - Detectors are different distances from sources
 - (Position of sources not perfectly reproduced each calibration)
 - Ratio of gamma line strengths will be different for each detector/calibration
 - One solution: create different normalised spectra for each gamma line?
- Not trivial to sum and fit
 - Poisson statistics must be treated correctly when adding events
- In future, could event combine spectra for multiple detectors for form dataset spectra

Conclusion

- GERDA searches for $0\nu\beta\beta$ of ^{76}Ge
- Regular calibrations are made with ^{228}Th sources
- Energy scale and resolution of detectors monitored
- Resolution at $Q_{\beta\beta}$ is determined by combining calibration spectra and detectors
- New method will produce more representative spectra