

# P2 status update

Anastasia Berdnikova

# cavern activities

## CW50


- Tues, 11 Dec      empty the cooling plant tank, start to remove cooling water from SMs and TS

## CW51

- Mon, 17 Dec      uncabbling of SMs
- Tues, 18 Dec      rotator installation, disconnection from gas system (only SM6)
- Wed, 19 Dec      extraction of SM6, installation in the clean room

# clean room status

- blue frame and rotator prepared by Bernd and his team
- heavy equipment moved to the cleanroom (Rittal rack, gas rack, 5 LV PS, CO2 bottle)

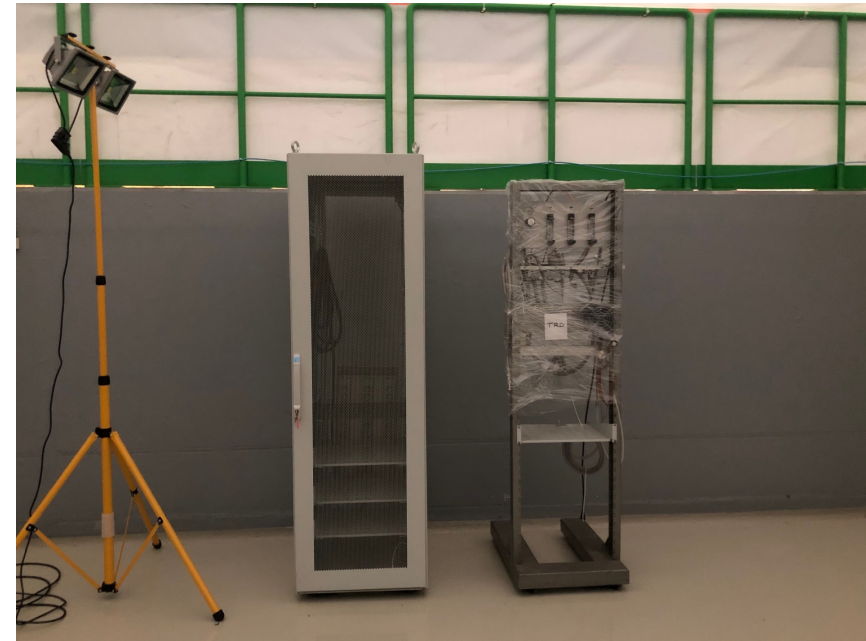

# open questions and suggestions

- which tests will be done at the cleanroom (it will define infrastructure which is needed)?
- can we use N<sub>2</sub> instead of CO<sub>2</sub>?
- if SM stays without flushing until January, closed with a filter – it is preferable to do a measurement of filter's impedance
- do we want to re-clean the cleanroom after SM installation?
- Database doesn't seem to be updated (at least regarding LV PS)